

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/25/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:17
INTERNAL STANDARD	VERIFIED	02:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:18
BLANK TEST	0.00	02:19
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:19
BLANK TEST	0.00	02:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:21
BLANK TEST	0.00	02:22

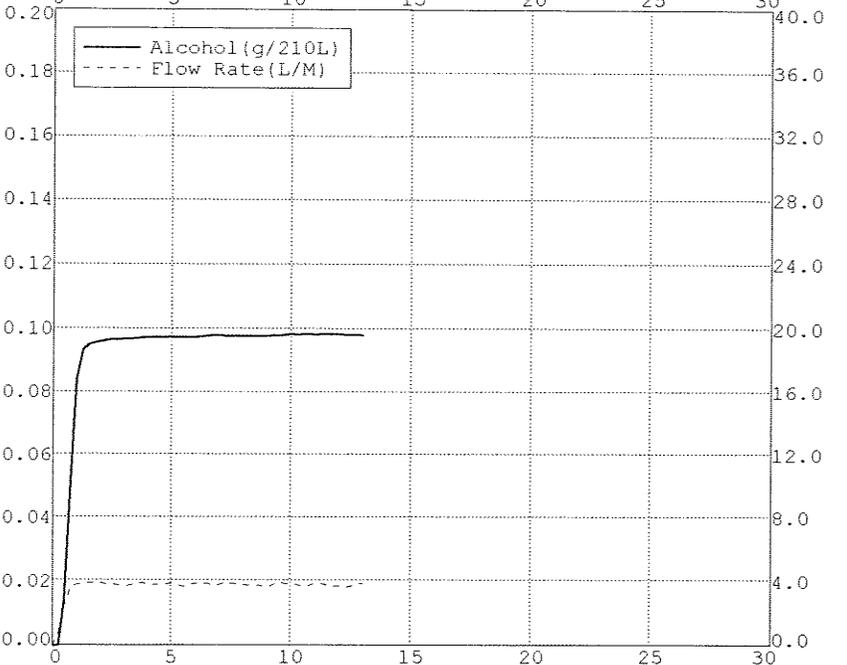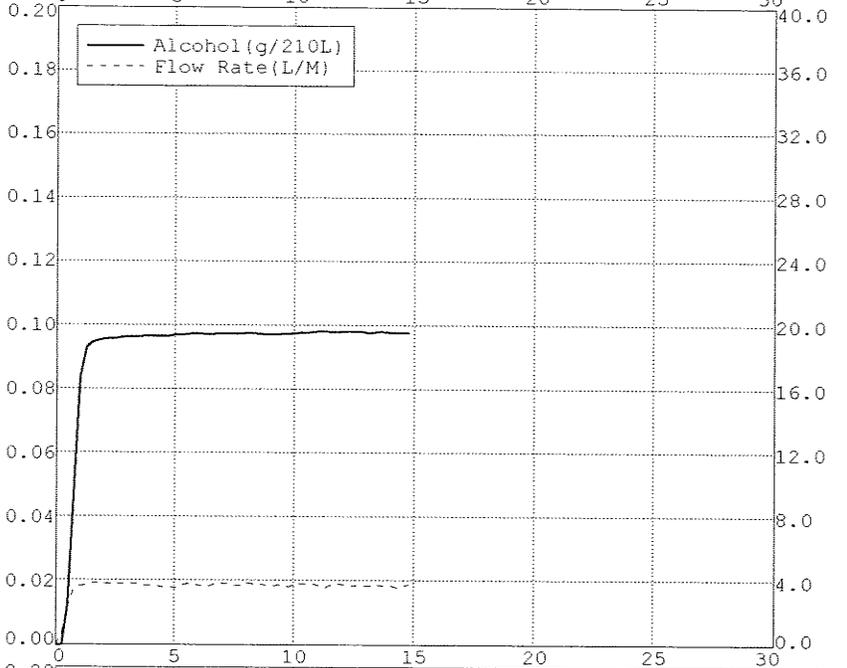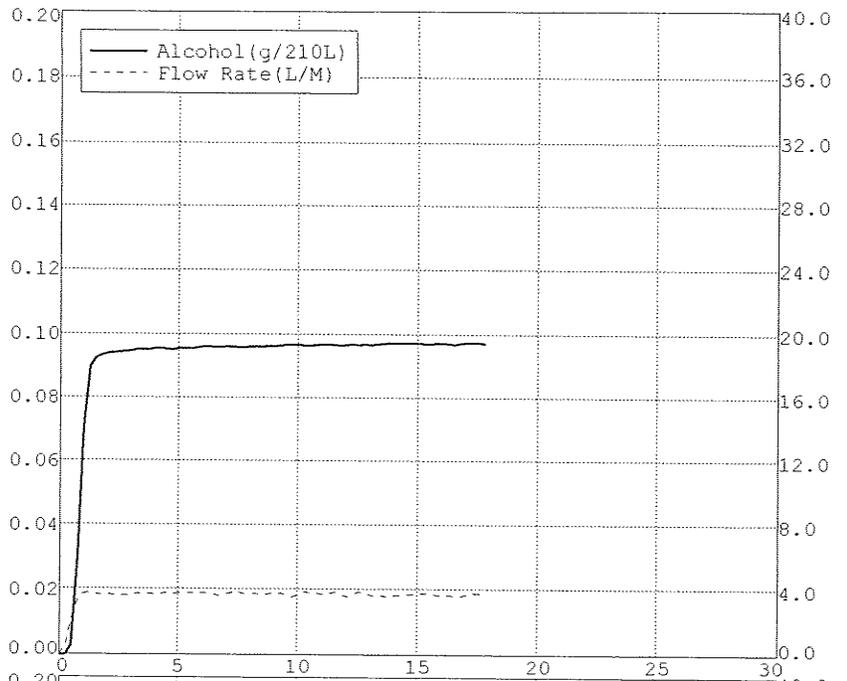

Charles B. Geisler #246