

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/21/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:10
INTERNAL STANDARD	VERIFIED	23:10
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	23:11
BLANK TEST	0.00	23:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:12
BLANK TEST	0.00	23:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:13
BLANK TEST	0.00	23:14

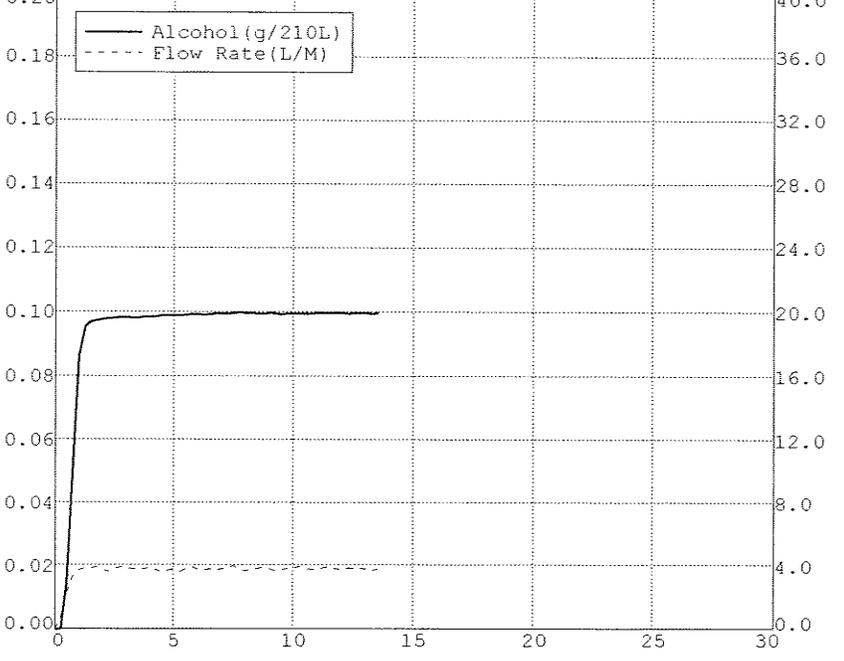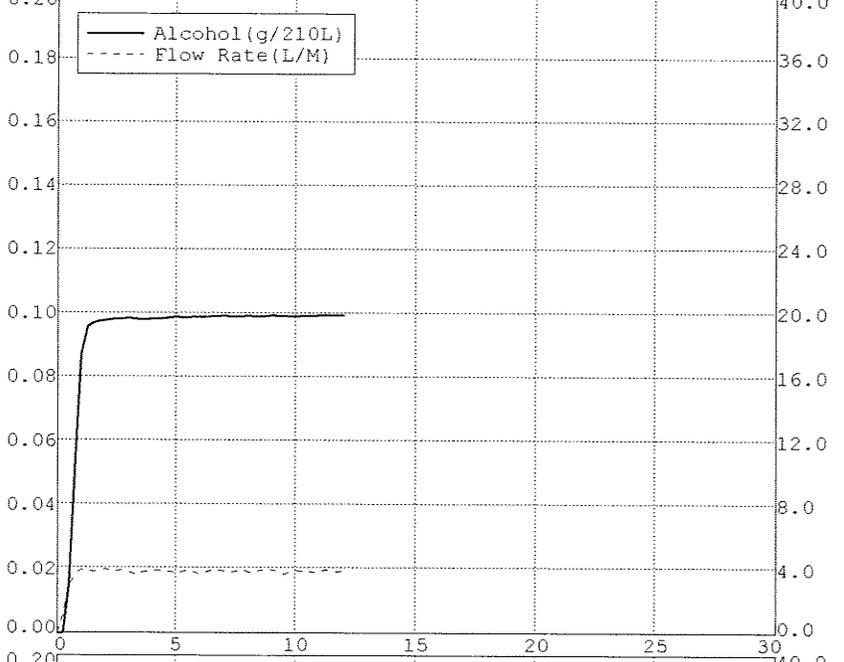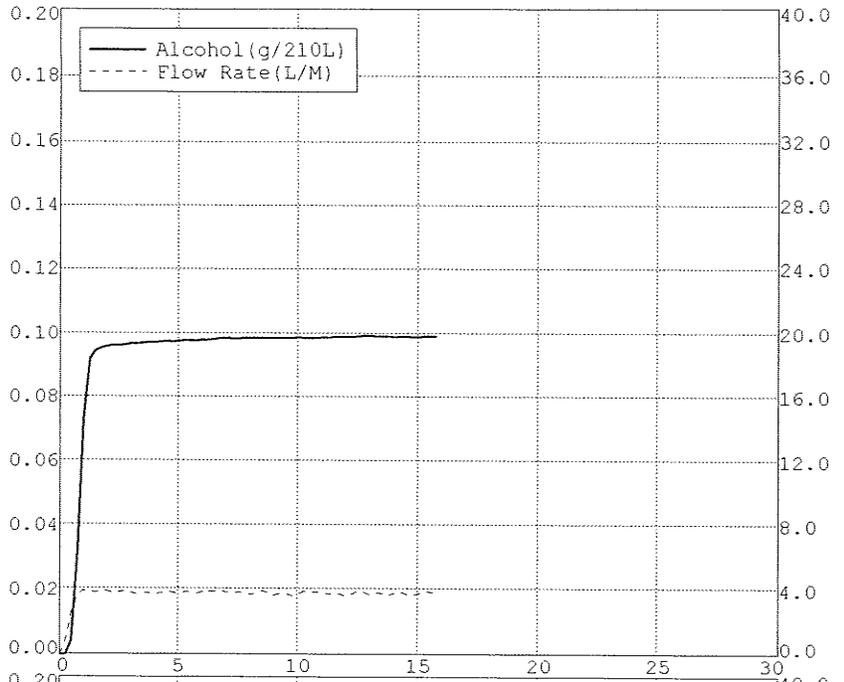

Sp. Chl B. Chl #246