

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/27/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:01
INTERNAL STANDARD	VERIFIED	22:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	22:02
BLANK TEST	0.00	22:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:03
BLANK TEST	0.00	22:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:04
BLANK TEST	0.00	22:05

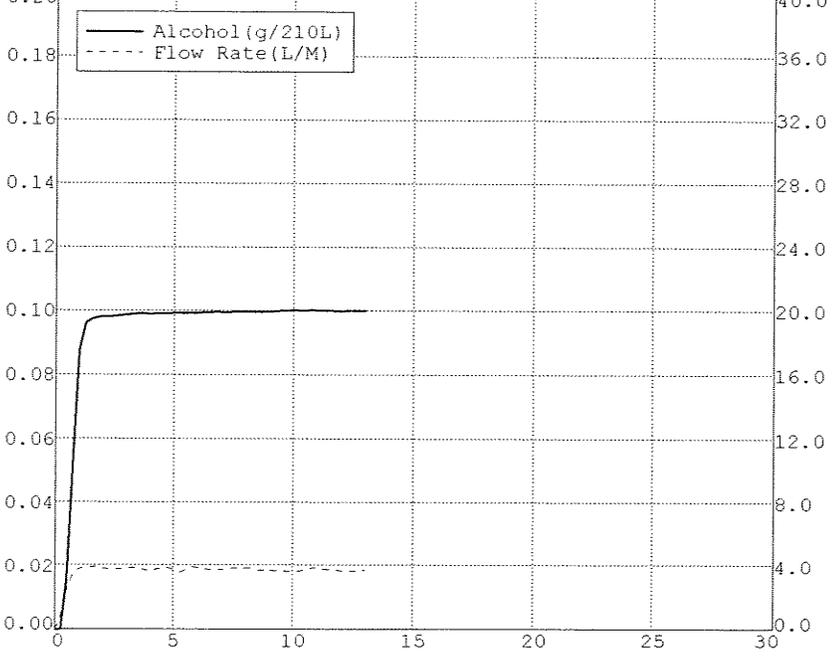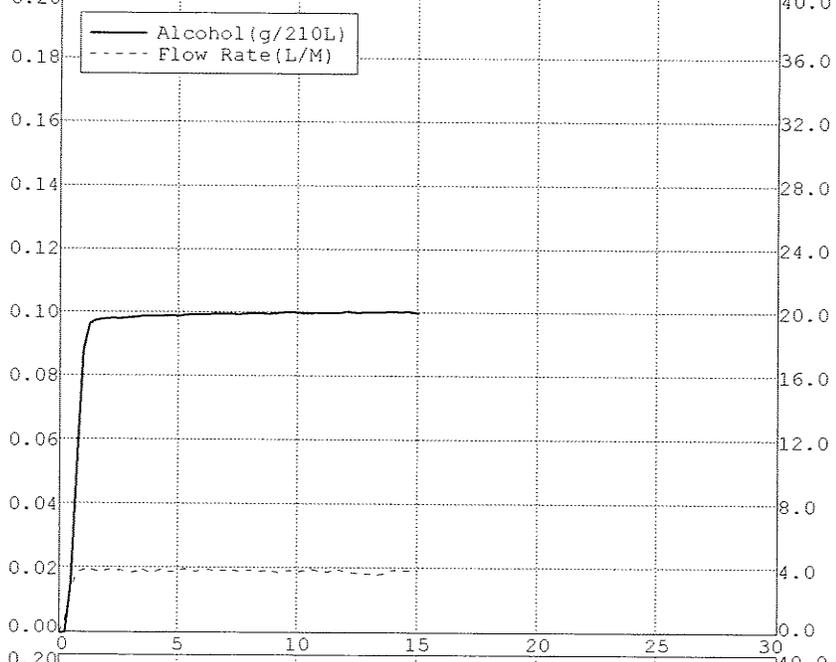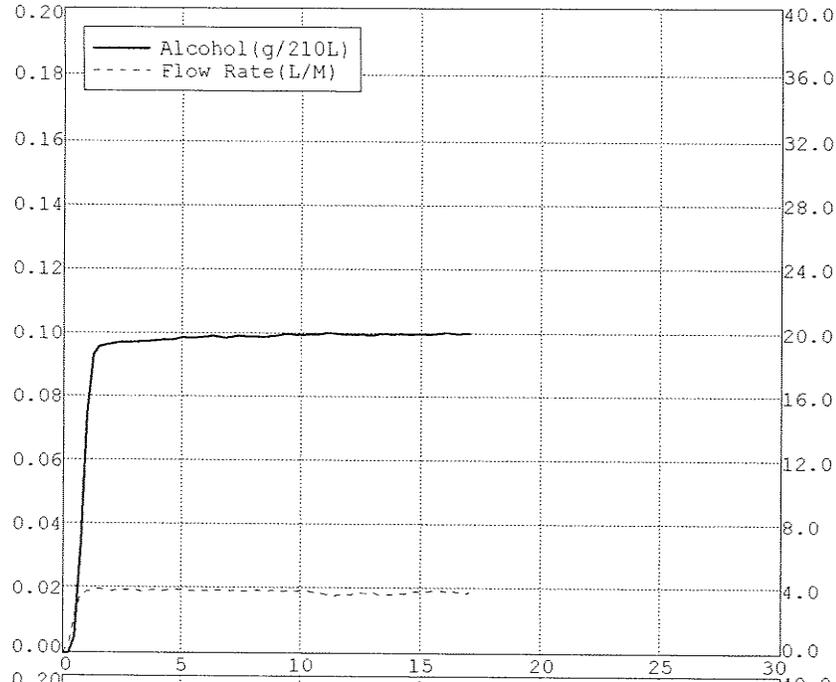

Sp. Chl. B. C. D. #2215