

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 09/08/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:44
INTERNAL STANDARD	VERIFIED	22:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:44
BLANK TEST	0.00	22:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:46
BLANK TEST	0.00	22:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:47
BLANK TEST	0.00	22:48

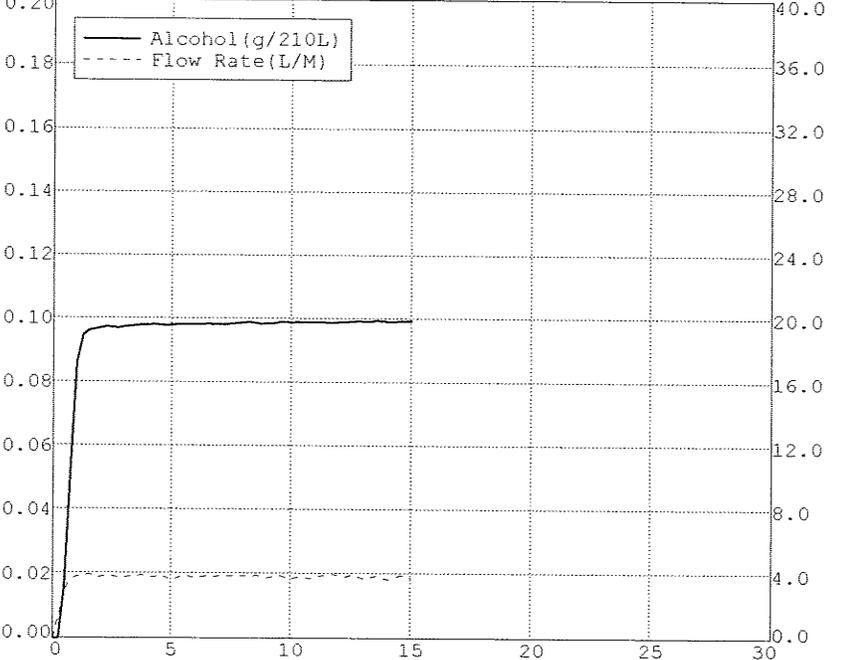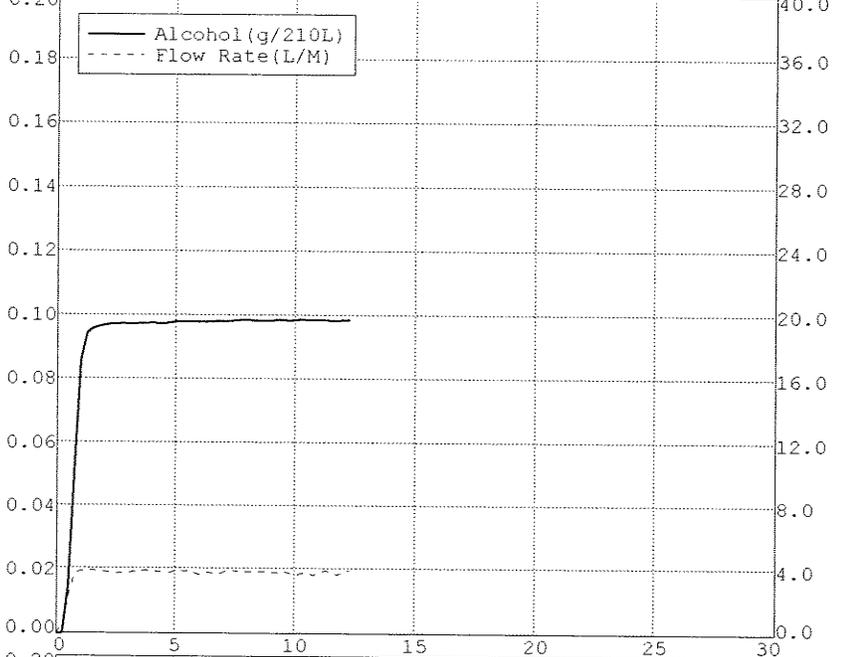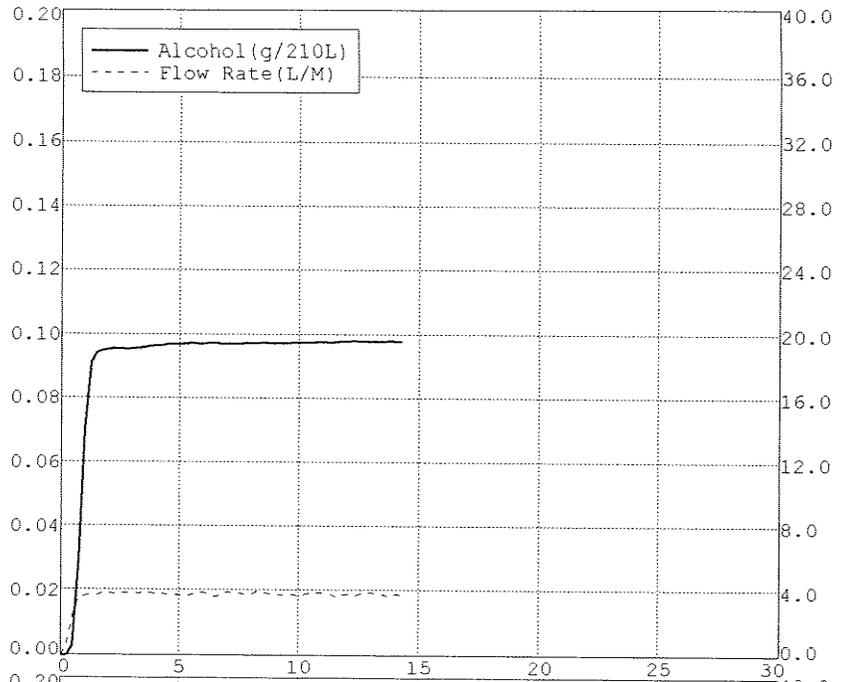

Charles B. Geisler #296