

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 09/13/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:03
INTERNAL STANDARD	VERIFIED	14:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:04
BLANK TEST	0.00	14:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:05
BLANK TEST	0.00	14:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:07
BLANK TEST	0.00	14:08

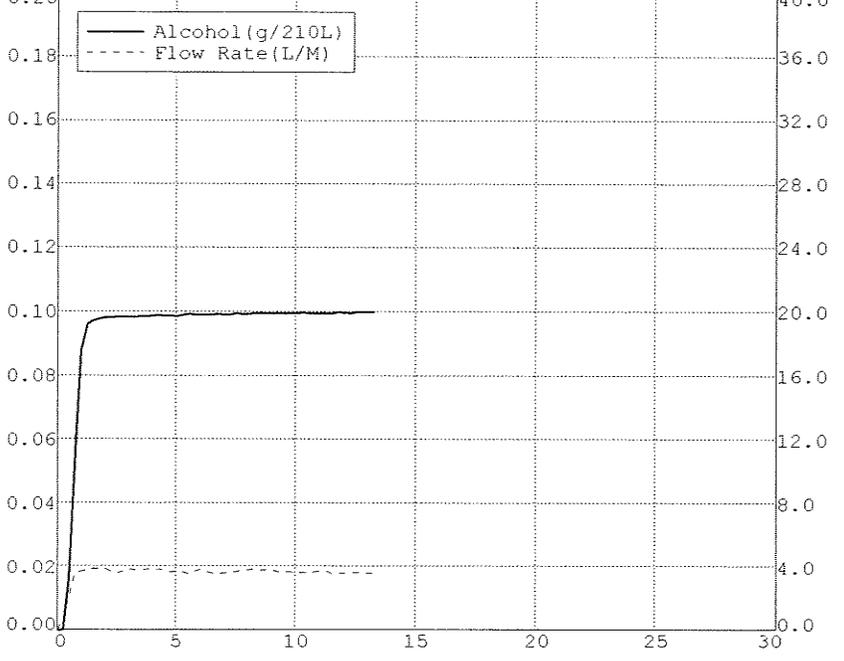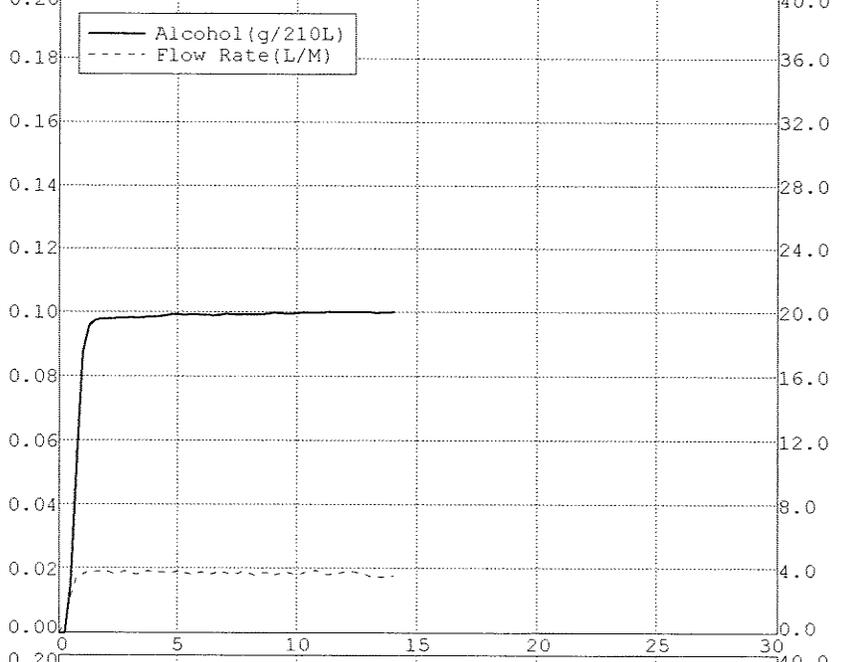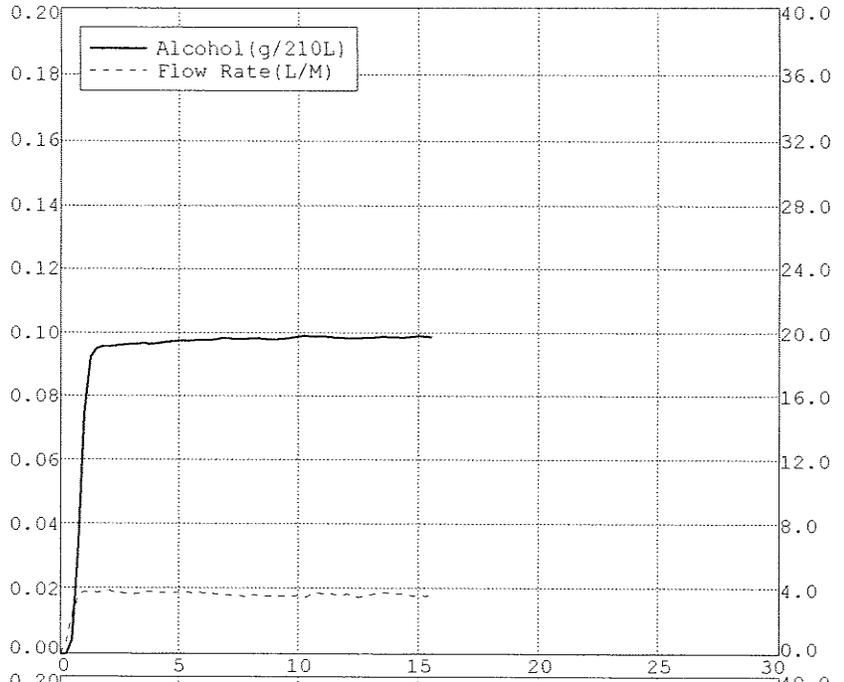

Charles B Geisler #241