

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 09/19/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN COUNTY
SHERIFF'S OFFICE
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:48
INTERNAL STANDARD	VERIFIED	02:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:49
BLANK TEST	0.00	02:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	02:50
BLANK TEST	0.00	02:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:52
BLANK TEST	0.00	02:53

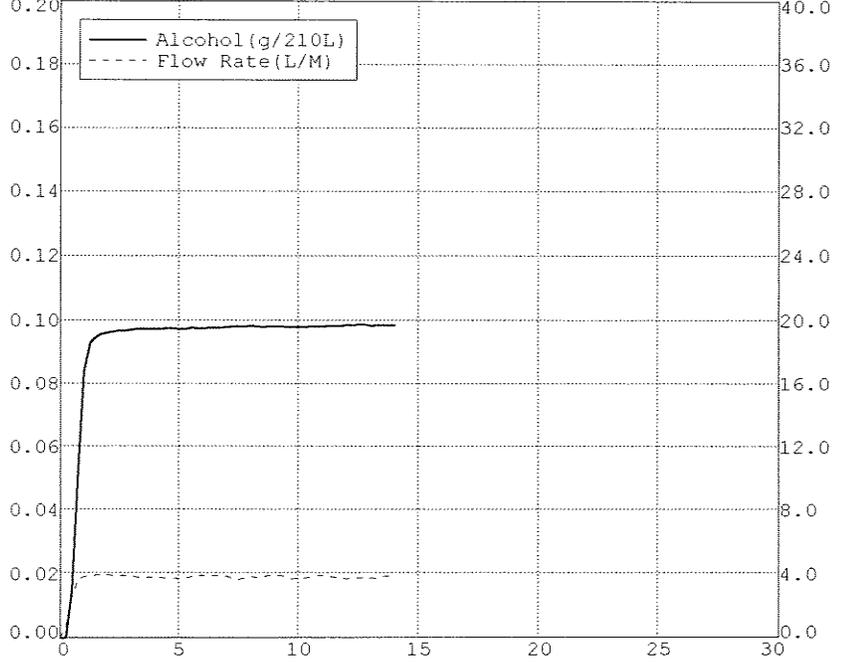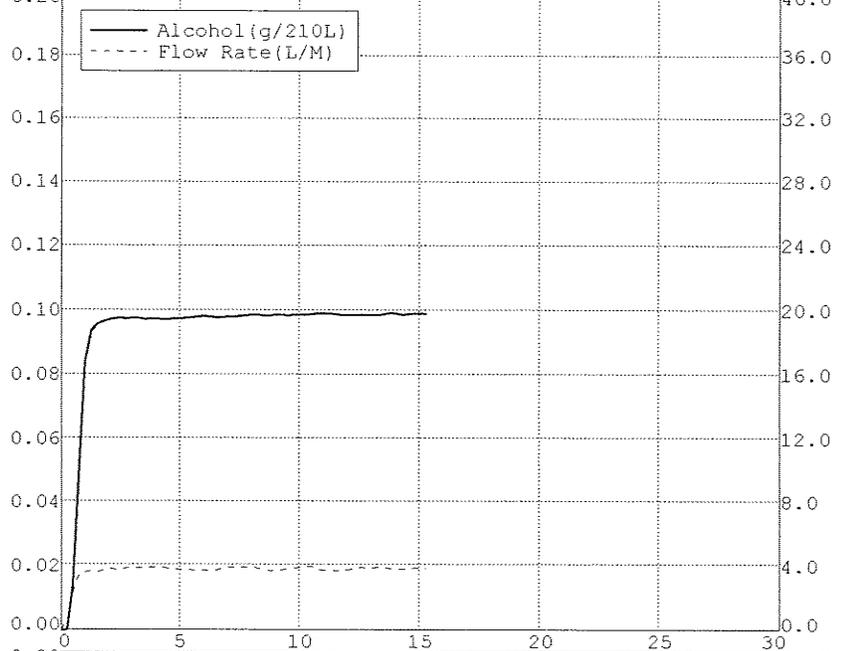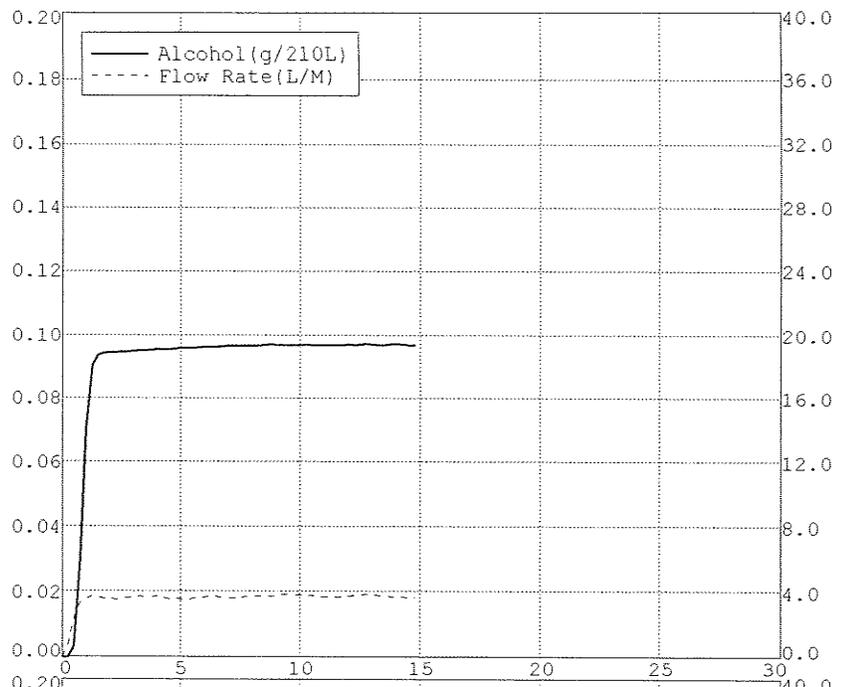

Ge. Charles B. Geisler #241