

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 09/25/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:52
INTERNAL STANDARD	VERIFIED	00:53
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:53
BLANK TEST	0.00	00:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:54
BLANK TEST	0.00	00:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:56
BLANK TEST	0.00	00:57

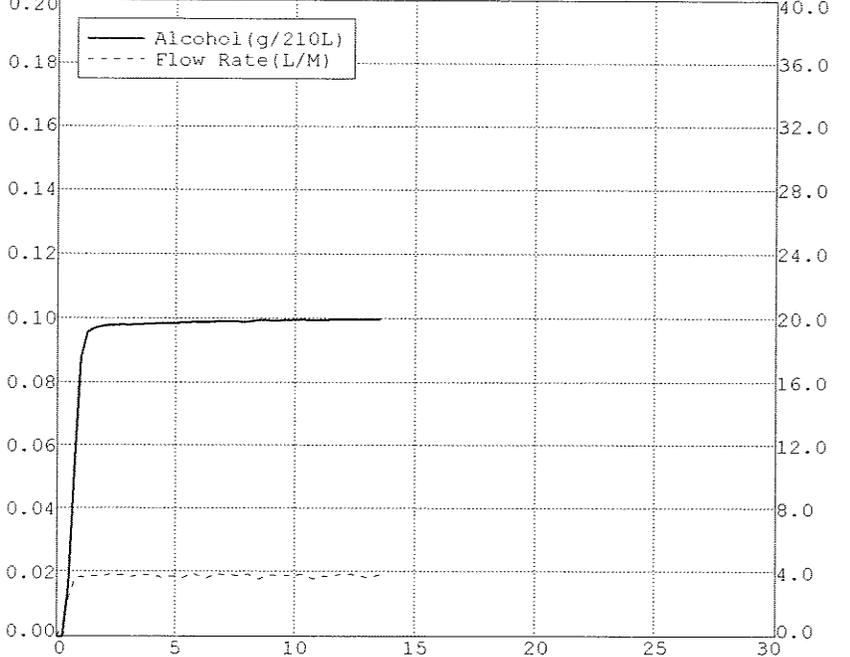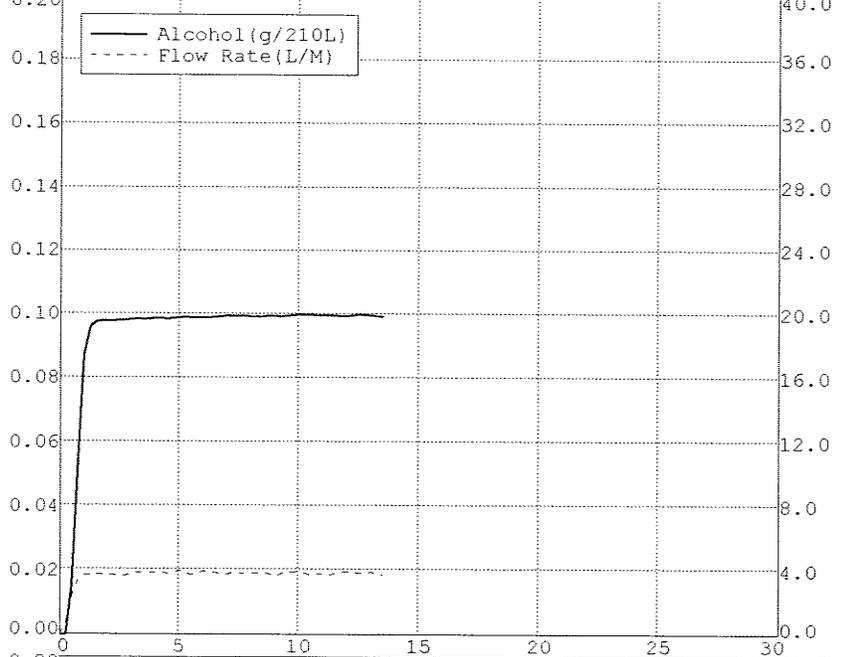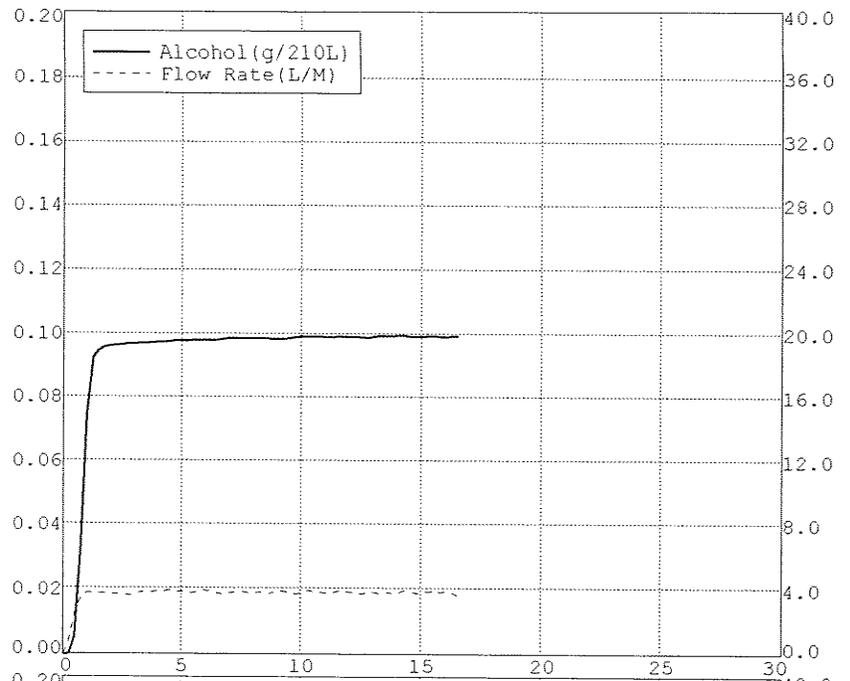

For Ch 175 R/L #245