

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 11/01/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:07
INTERNAL STANDARD	VERIFIED	16:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:07
BLANK TEST	0.00	16:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:09
BLANK TEST	0.00	16:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:10
BLANK TEST	0.00	16:11

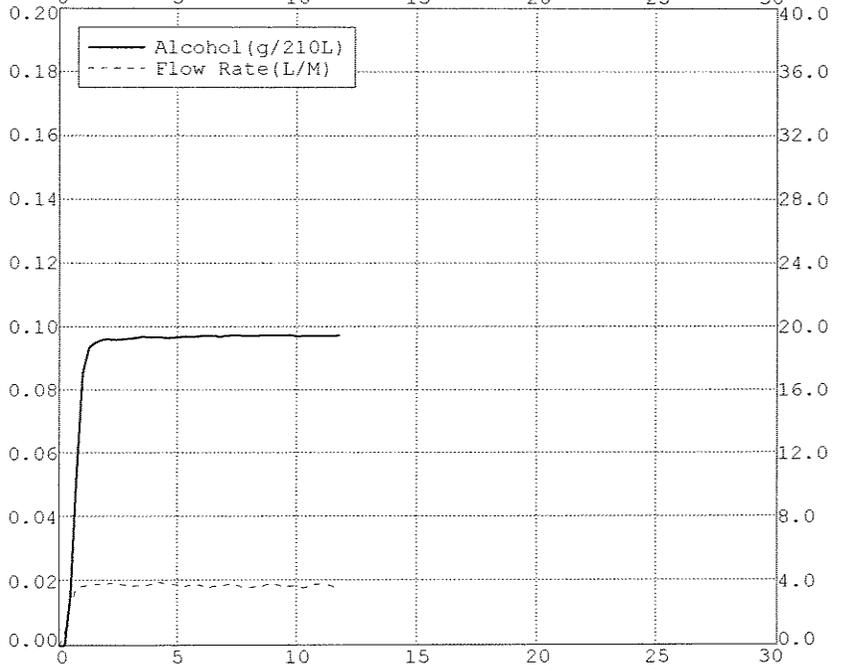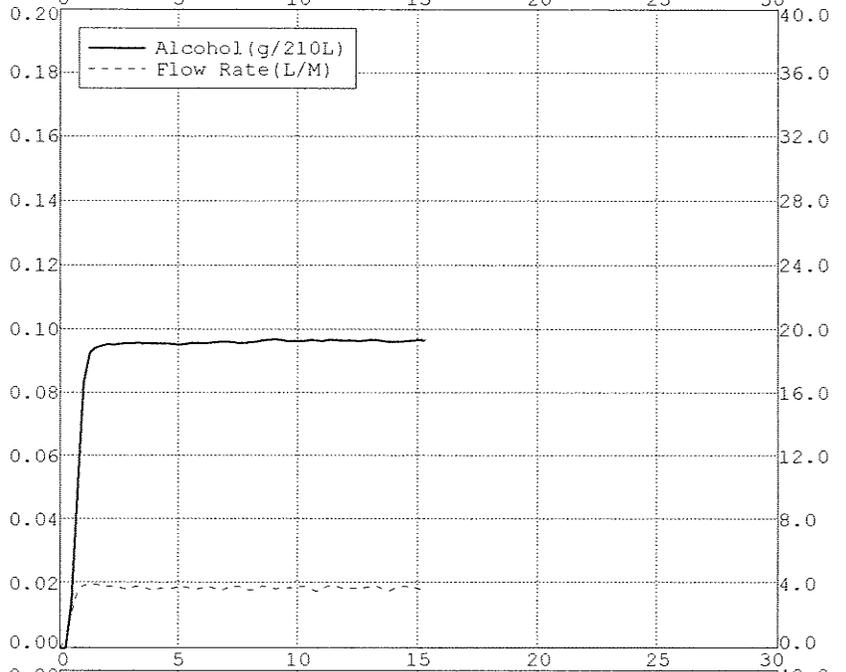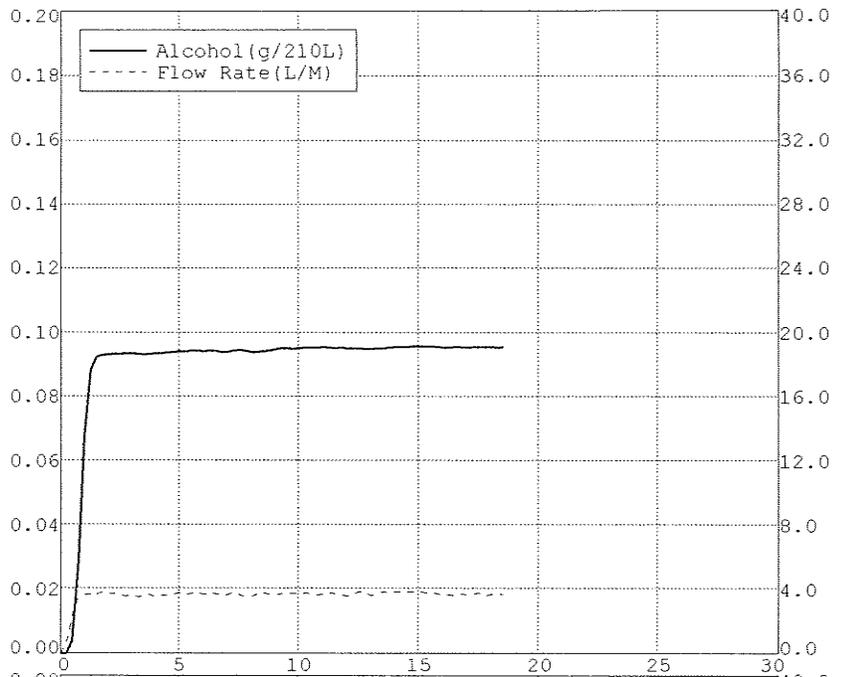

*Ch. B. Geisler* #211