

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 11/07/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:50
INTERNAL STANDARD	VERIFIED	11:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	11:51
BLANK TEST	0.00	11:52
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	11:52
BLANK TEST	0.00	11:53
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	11:54
BLANK TEST	0.00	11:55

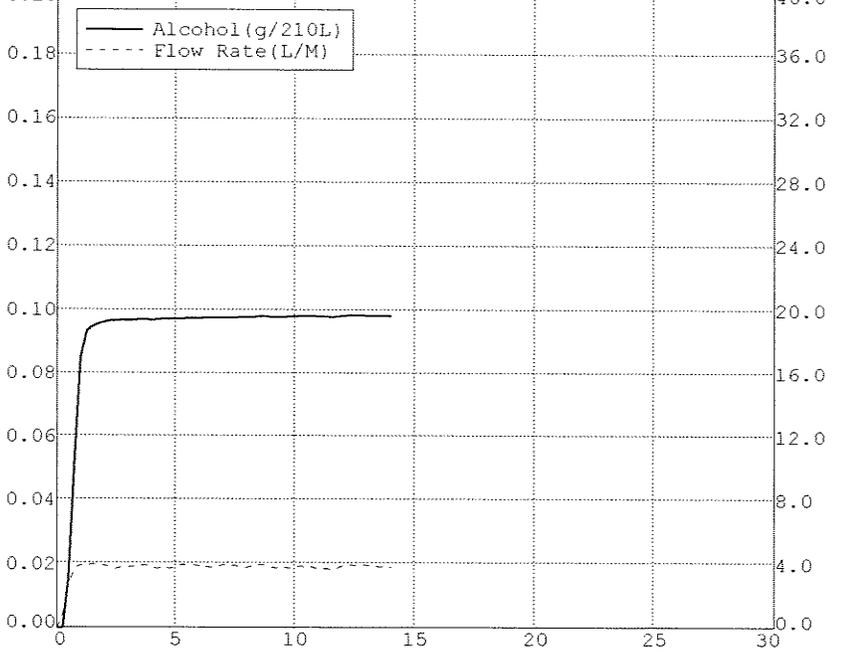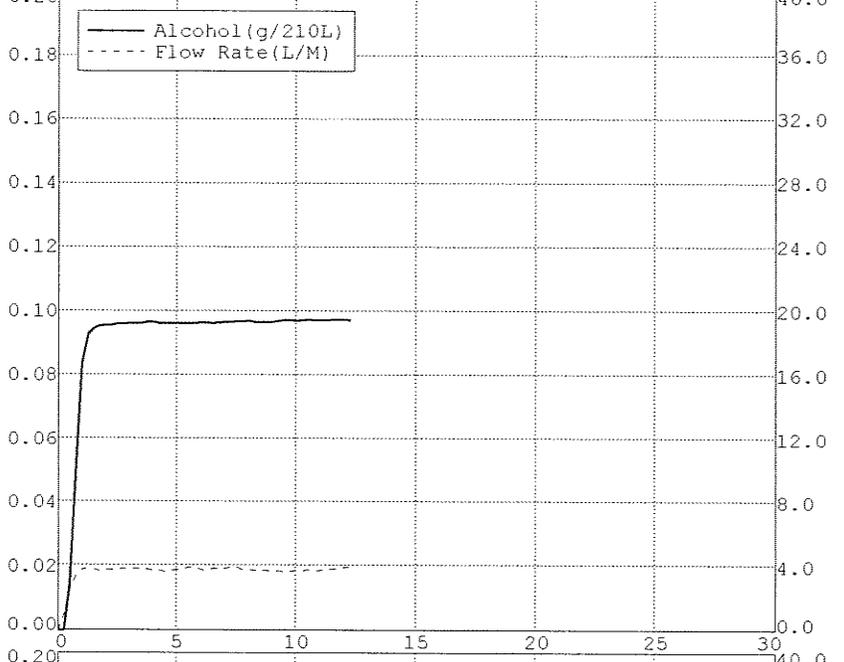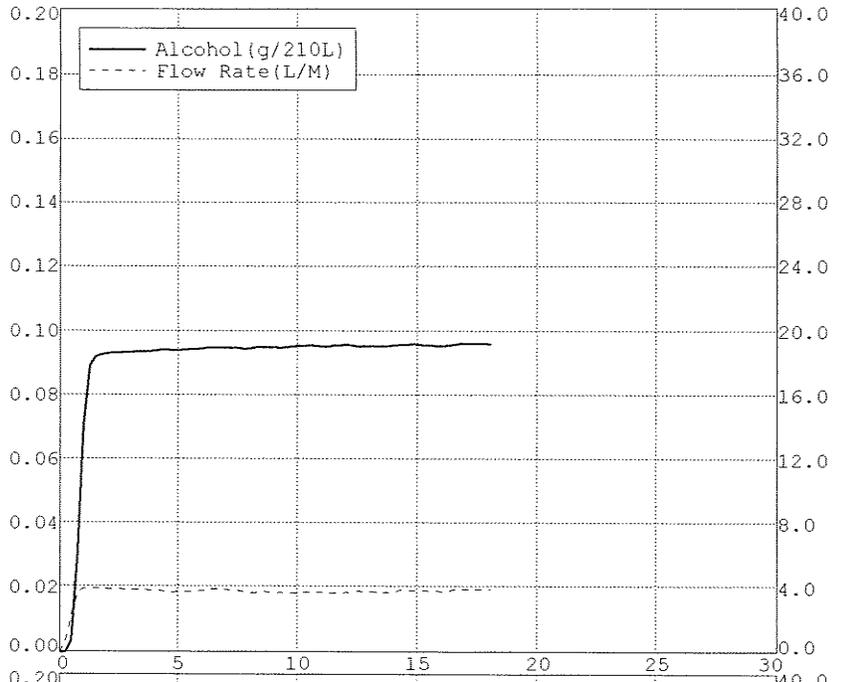

*Charles B Geisler #2211*