

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/20/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:31
INTERNAL STANDARD	VERIFIED	03:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:31
BLANK TEST	0.00	03:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:32
BLANK TEST	0.00	03:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:34
BLANK TEST	0.00	03:35

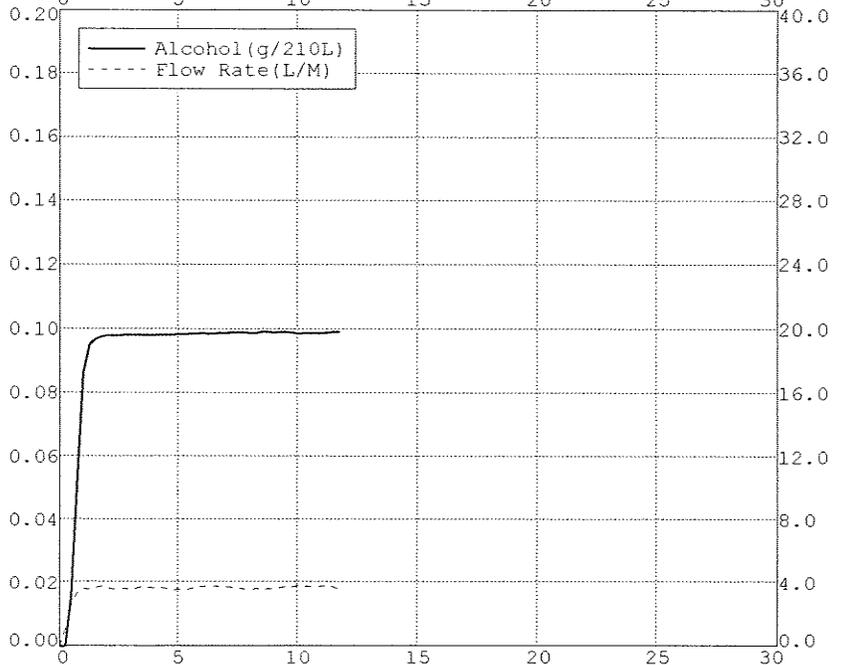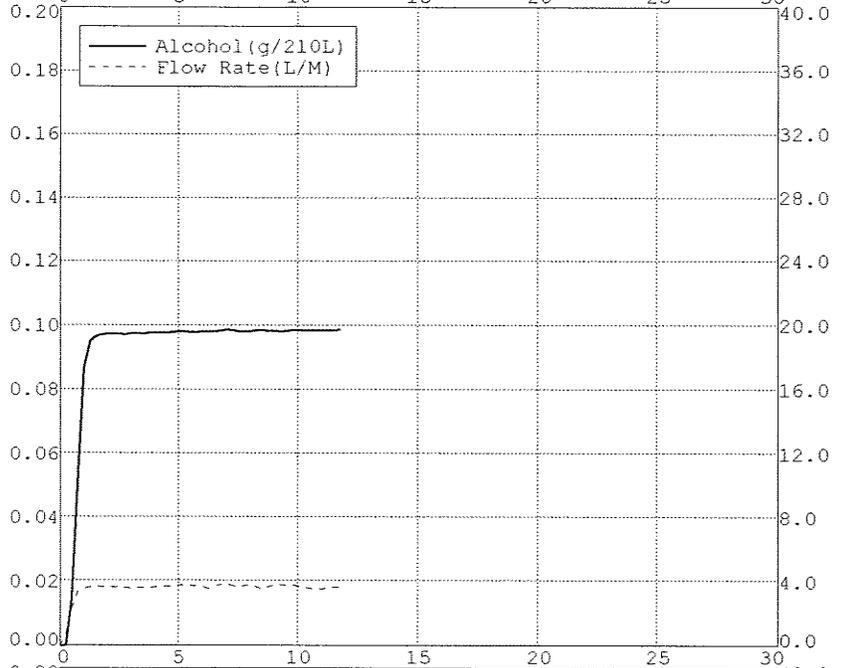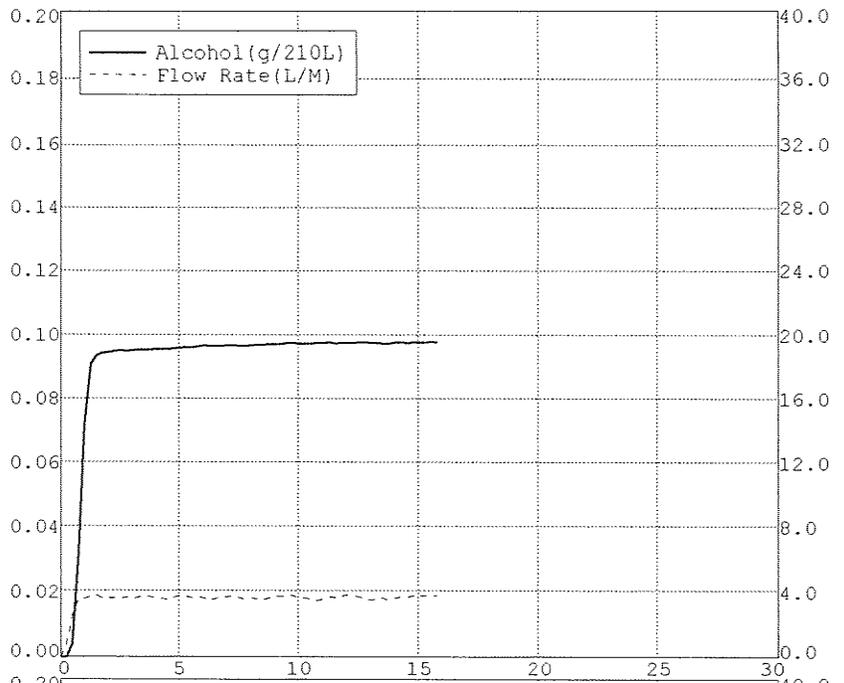

Charles B. Geisler #214