

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/27/2017

OPERATOR NAME:
TYLER J MORSE
Permit #: 41959
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:33
INTERNAL STANDARD	VERIFIED	09:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:34
BLANK TEST	0.00	09:35
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	09:35
BLANK TEST	0.00	09:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:36
BLANK TEST	0.00	09:37

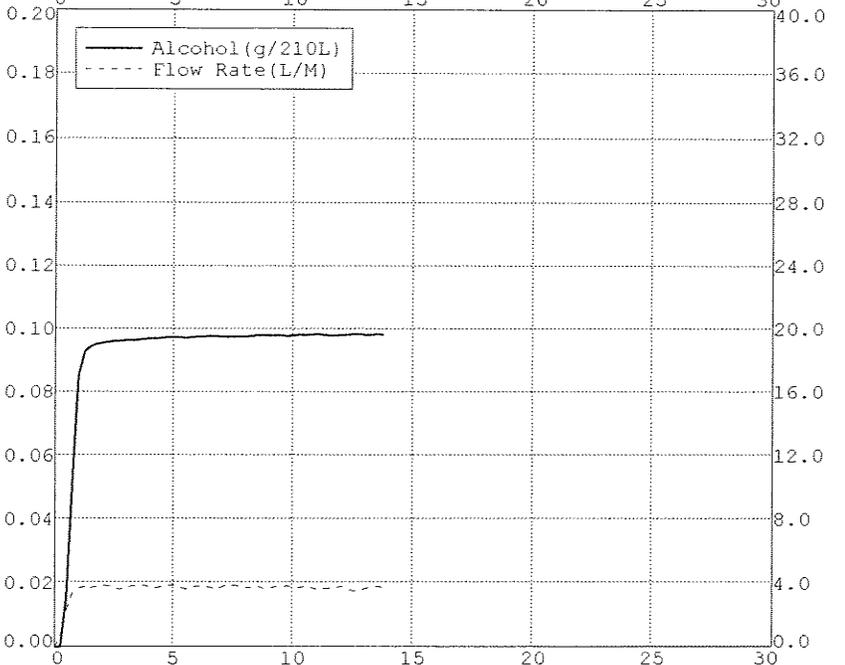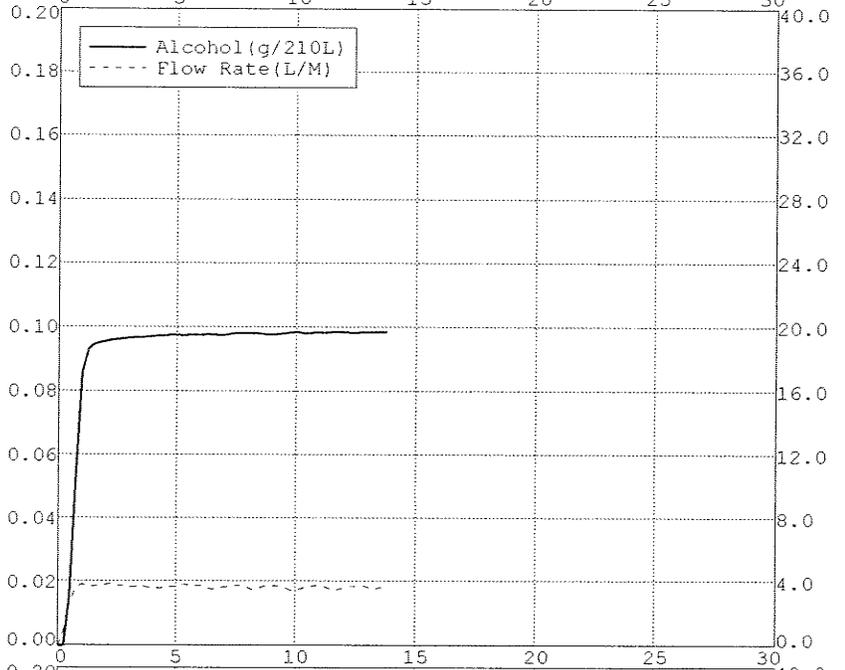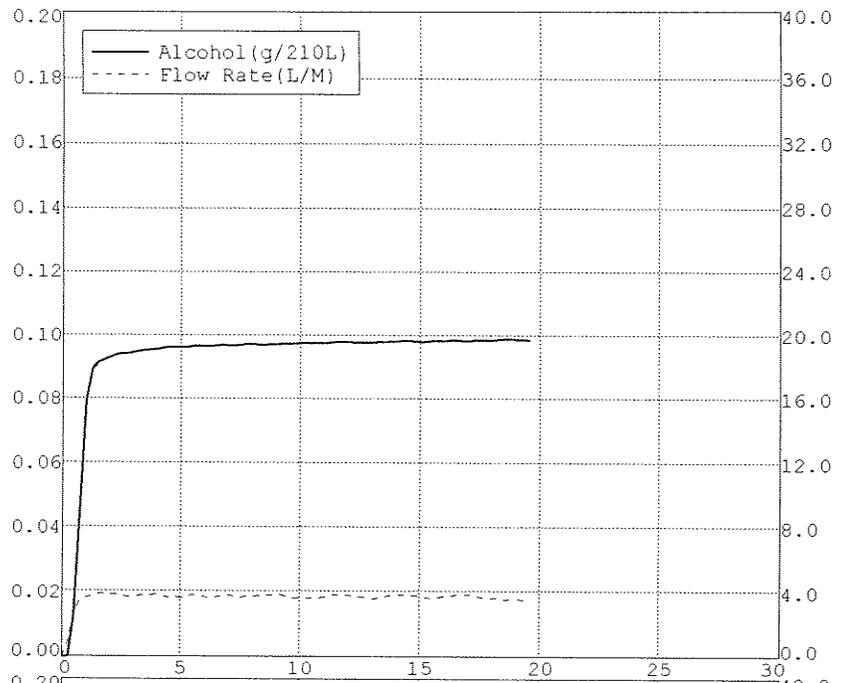

Ph #1417