

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 01/02/2017

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16240

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:13
INTERNAL STANDARD	VERIFIED	00:13
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	00:13
BLANK TEST	0.00	00:14
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	00:15
BLANK TEST	0.00	00:16
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	00:16
BLANK TEST	0.00	00:17

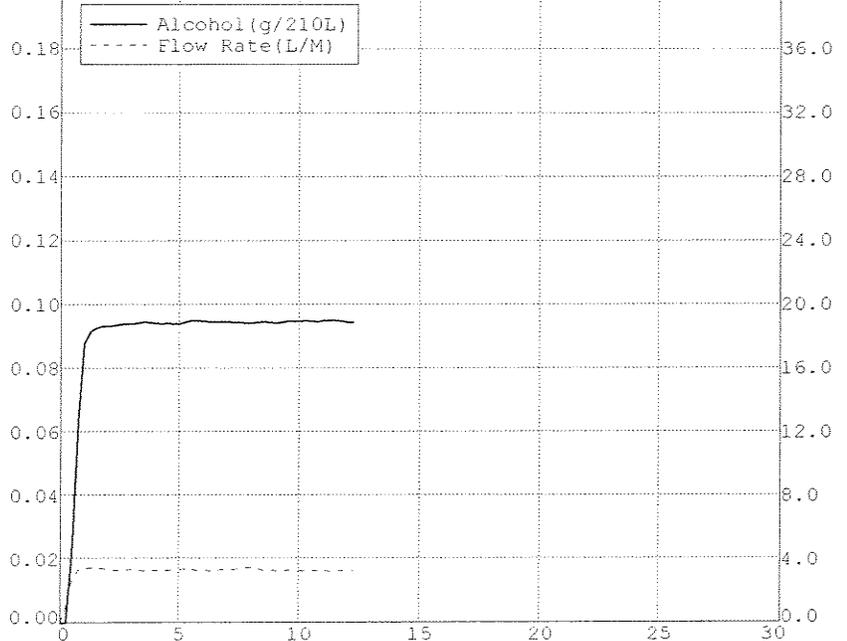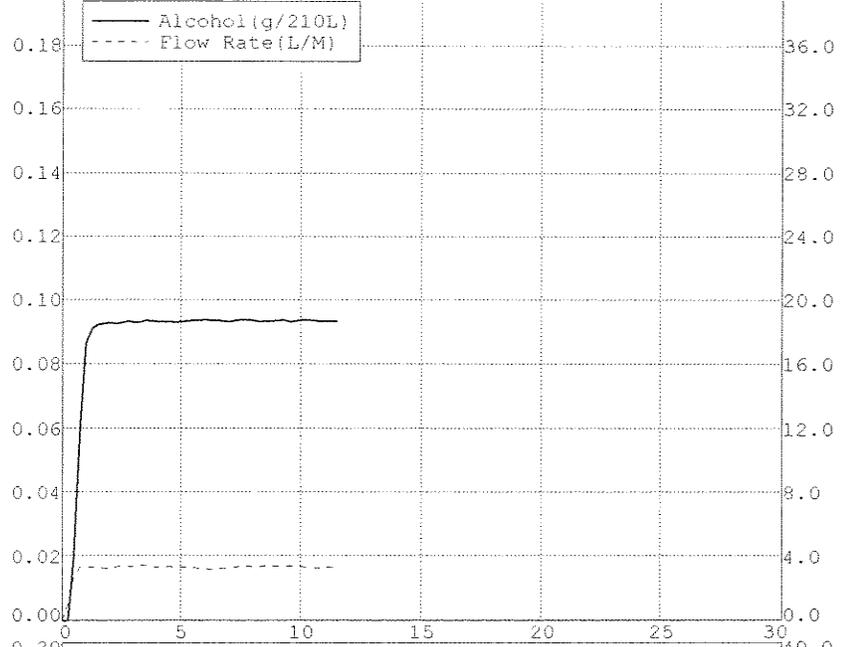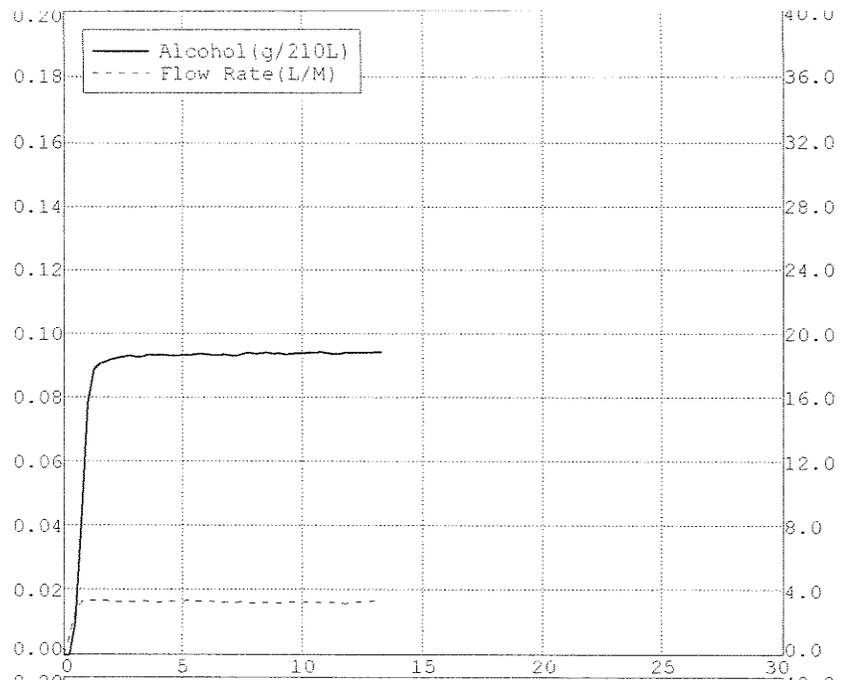

SGS by *Rutledge* WESU #162  
01/02/17