

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 01/10/2017

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16240

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:08
INTERNAL STANDARD	VERIFIED	00:08
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:08
BLANK TEST	0.00	00:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:09
BLANK TEST	0.00	00:10
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:10
BLANK TEST	0.00	00:11

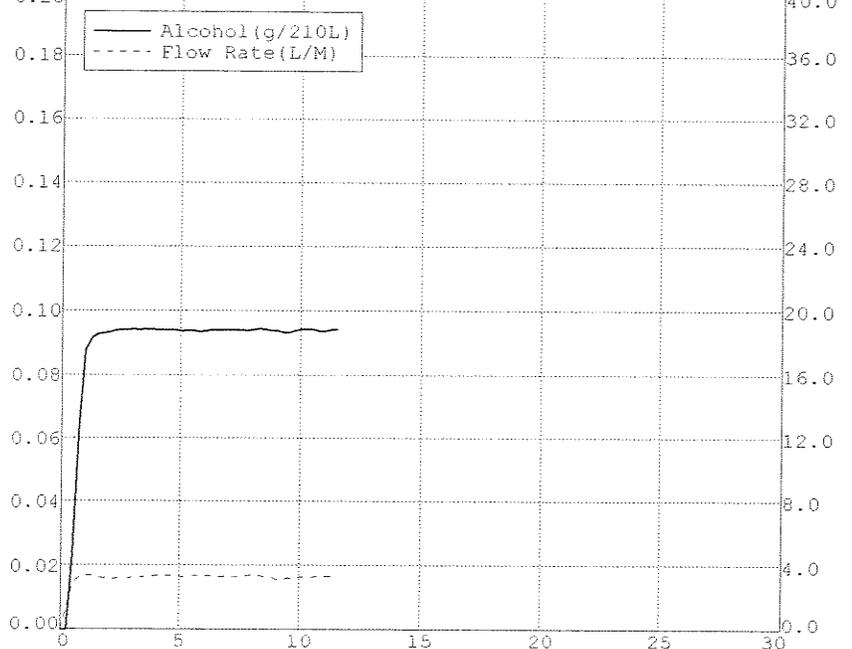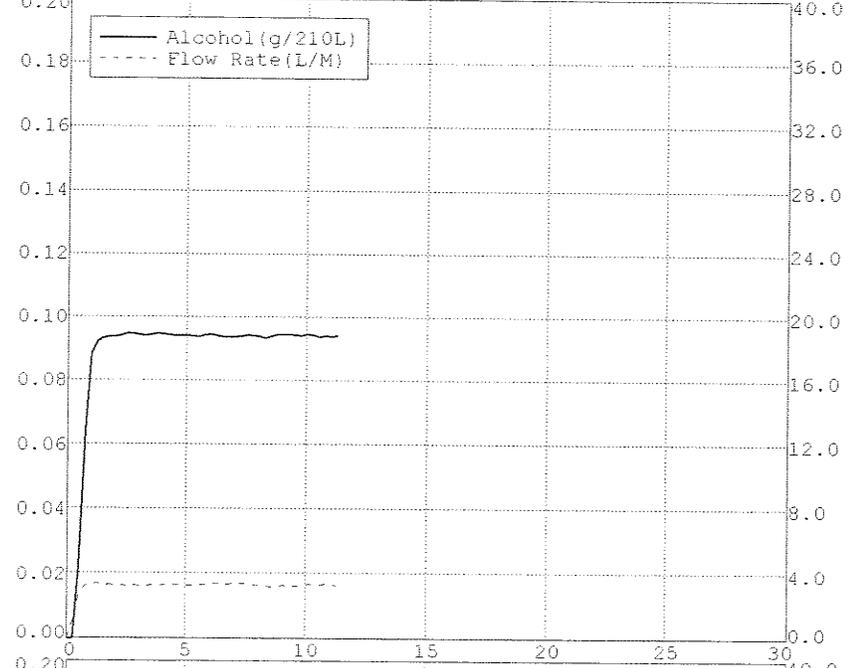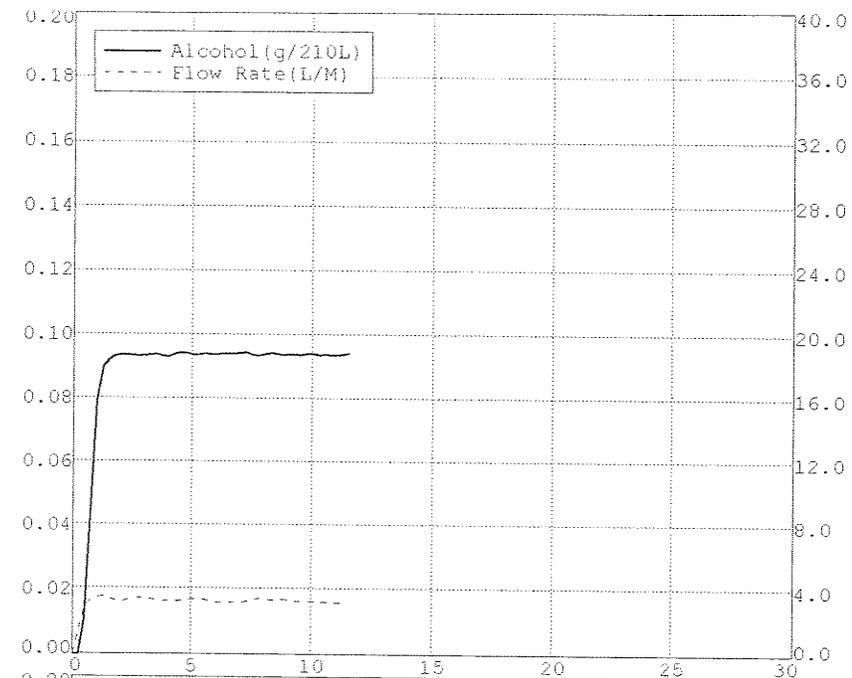

SES *RJ Bartlett* WESU #102

01-10-17