

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/16/2017

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16240

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:18
INTERNAL STANDARD	VERIFIED	00:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:19
BLANK TEST	0.00	00:20
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:20
BLANK TEST	0.00	00:21
REFERENCE STANDARD TEMP	33.93c	
REFERENCE STANDARD	0.09	00:21
BLANK TEST	0.00	00:22

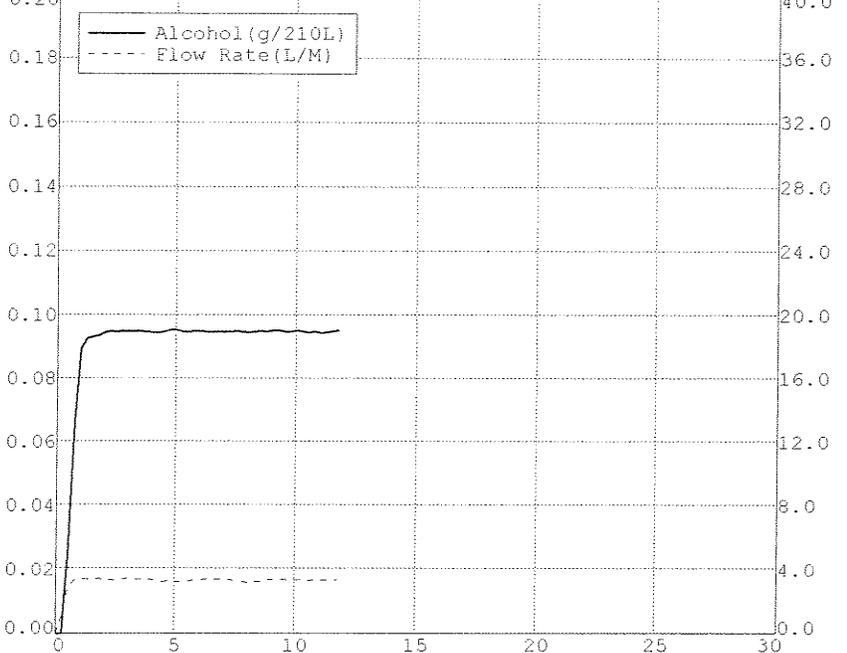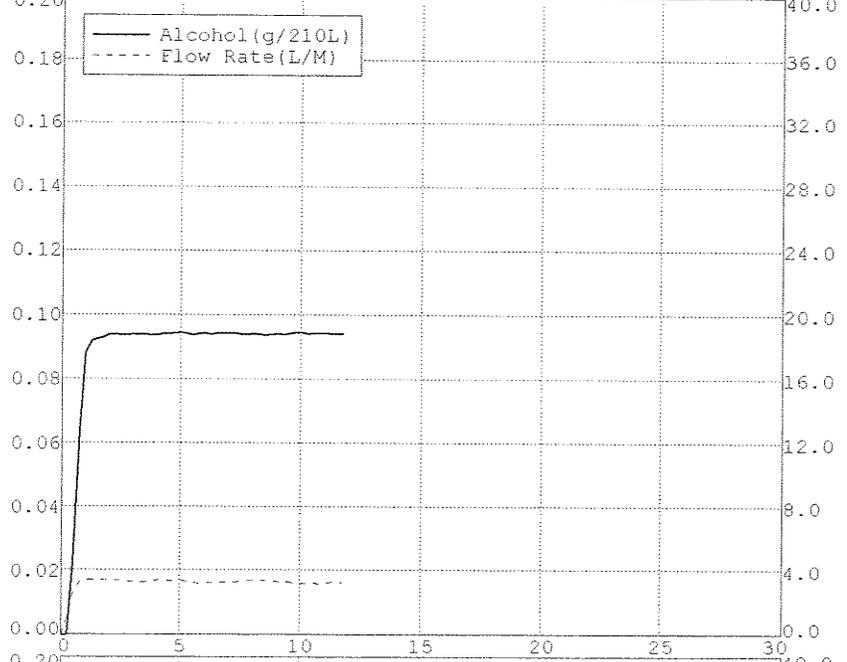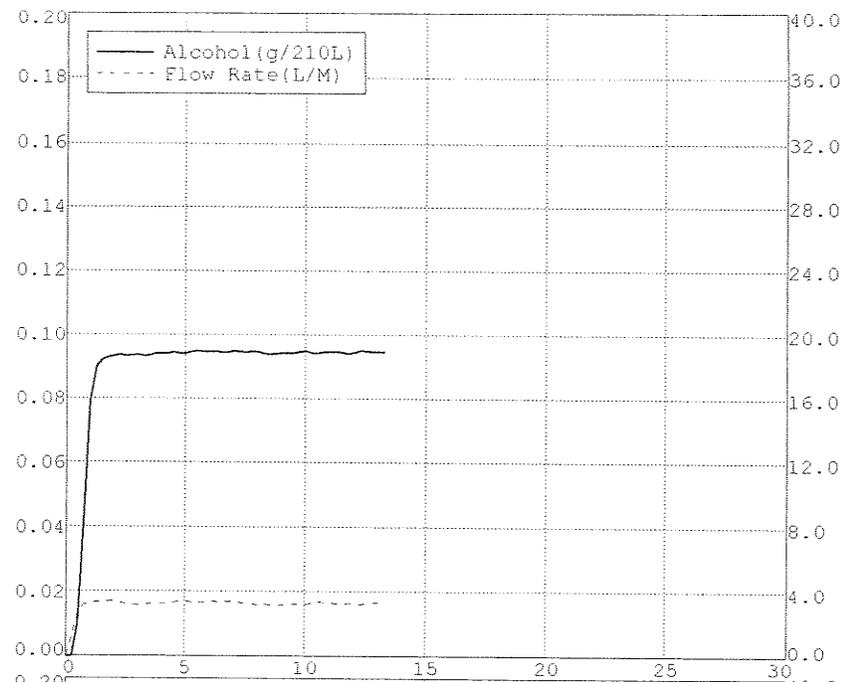

SGT R.J. Bartlett WCSI #162

01-16-17