

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 02/13/2017

OPERATOR NAME:  
 RALPH J BARTLETT  
 Permit #: 26222  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 16380

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:04
INTERNAL STANDARD	VERIFIED	03:04
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	03:04
BLANK TEST	0.00	03:05
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:05
BLANK TEST	0.00	03:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:07
BLANK TEST	0.00	03:08

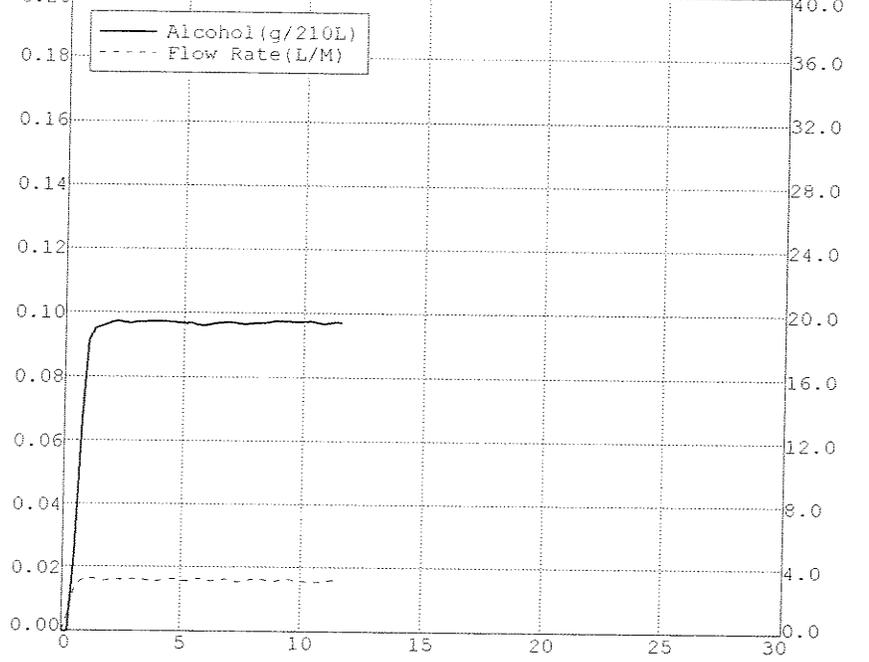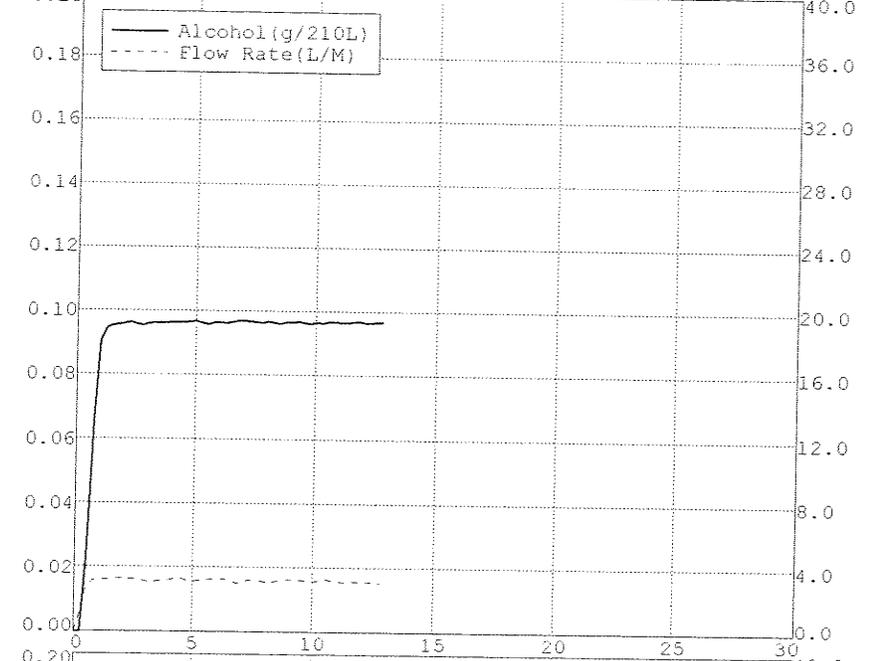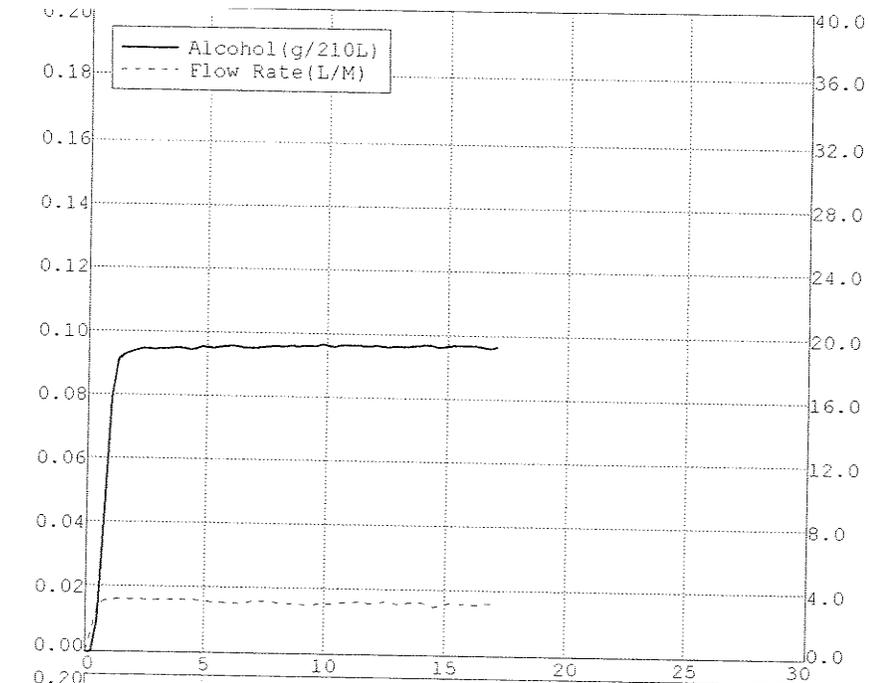

SGT *RJ Bartlett* WOSO #162

02-13-17