

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/21/2017

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16380

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:27
INTERNAL STANDARD	VERIFIED	00:27
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	00:27
BLANK TEST	0.00	00:28
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	00:28
BLANK TEST	0.00	00:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:30
BLANK TEST	0.00	00:31

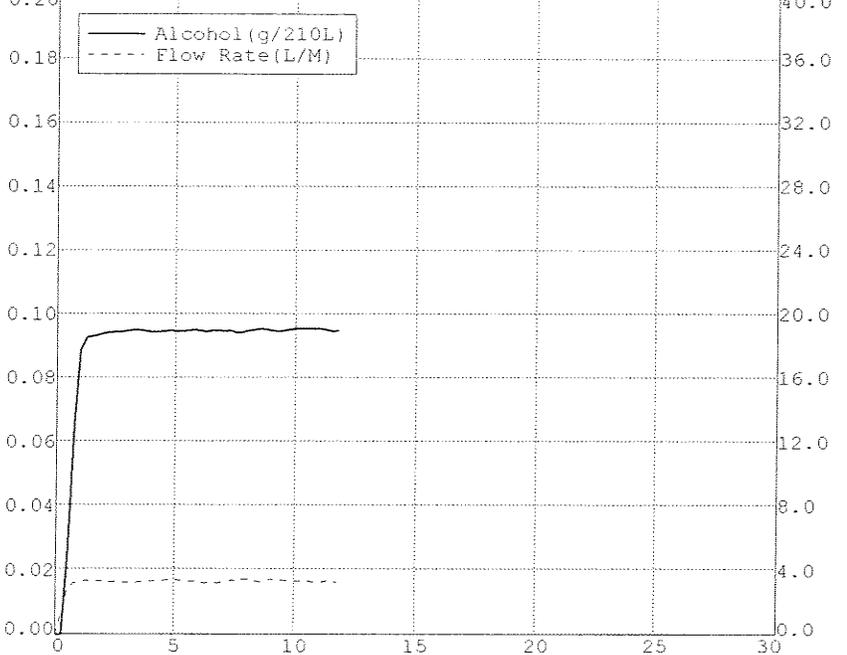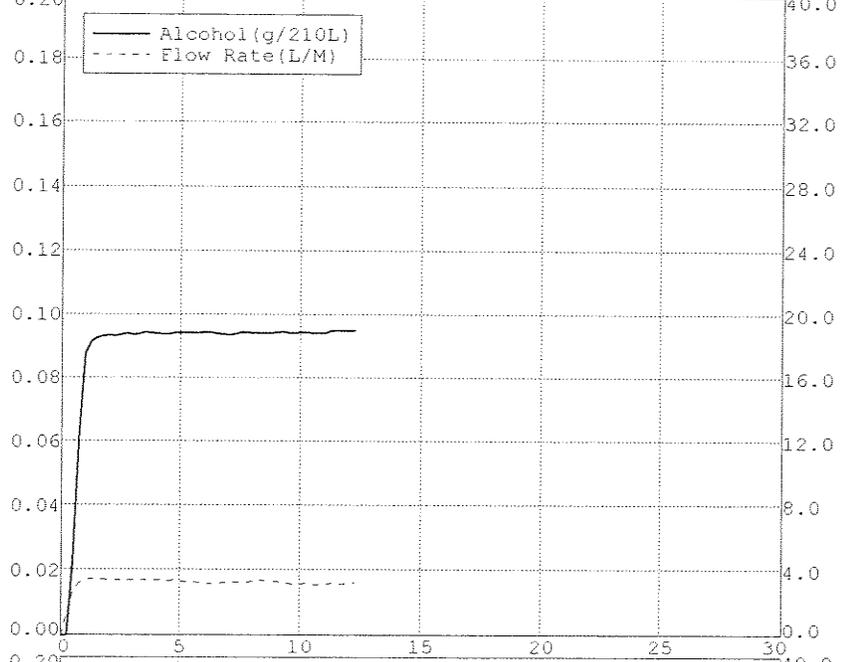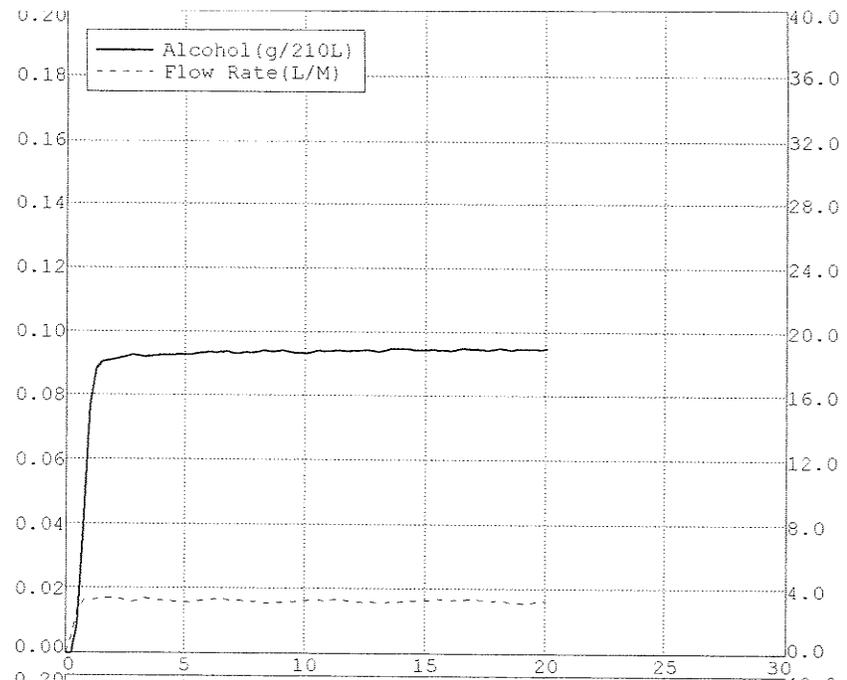

Sgt R.J. Bartlett WCSO #162
02-21-17