

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/26/2017

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16380

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:09
INTERNAL STANDARD	VERIFIED	23:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:10
BLANK TEST	0.00	23:11
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	23:11
BLANK TEST	0.00	23:12
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	23:12
BLANK TEST	0.00	23:13

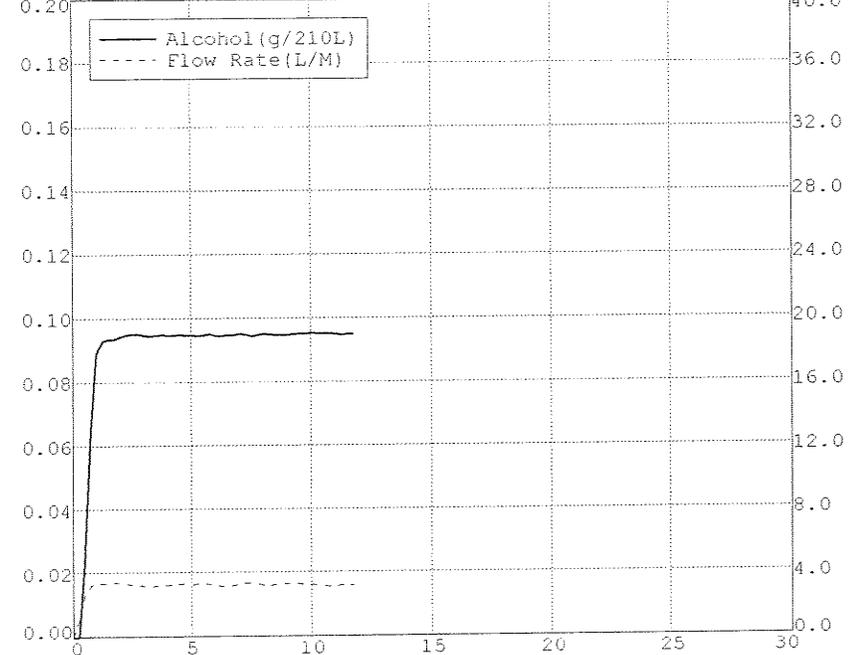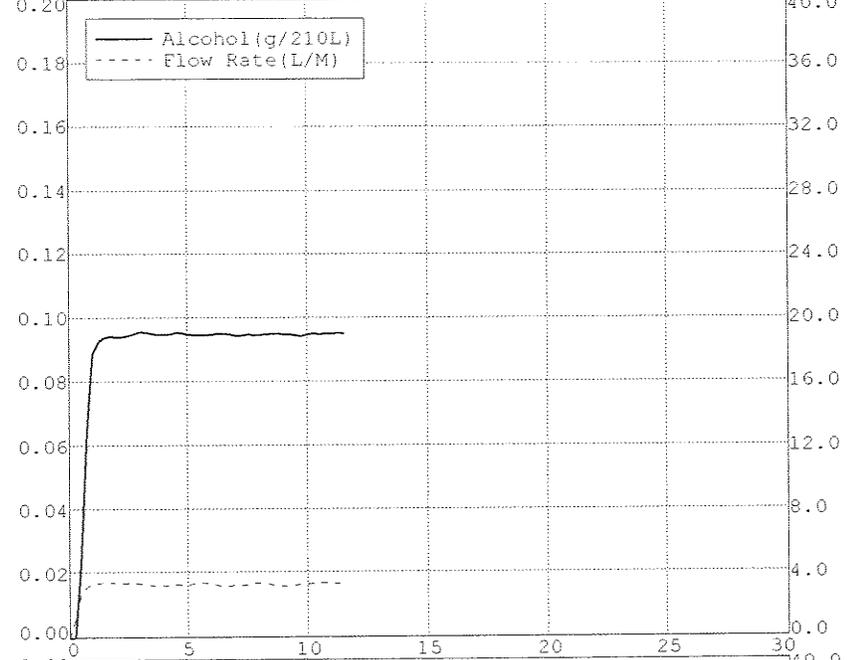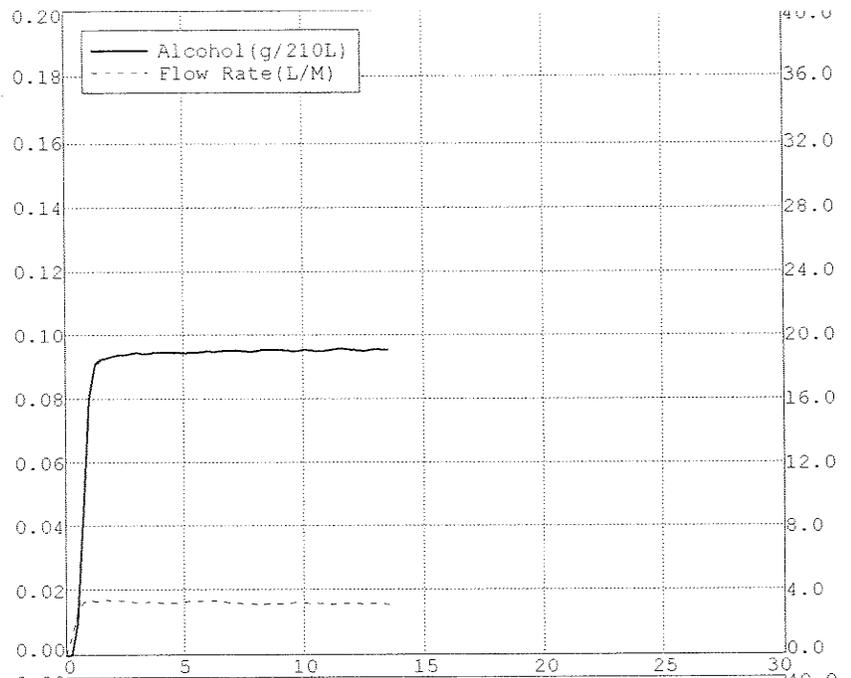

SGS *RJ Bartlett*
WSSO #162 02-26-17