

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 03/15/2017

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16380

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:30
INTERNAL STANDARD	VERIFIED	22:30
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	22:31
BLANK TEST	0.00	22:31
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	22:32
BLANK TEST	0.00	22:33
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	22:33
BLANK TEST	0.00	22:34

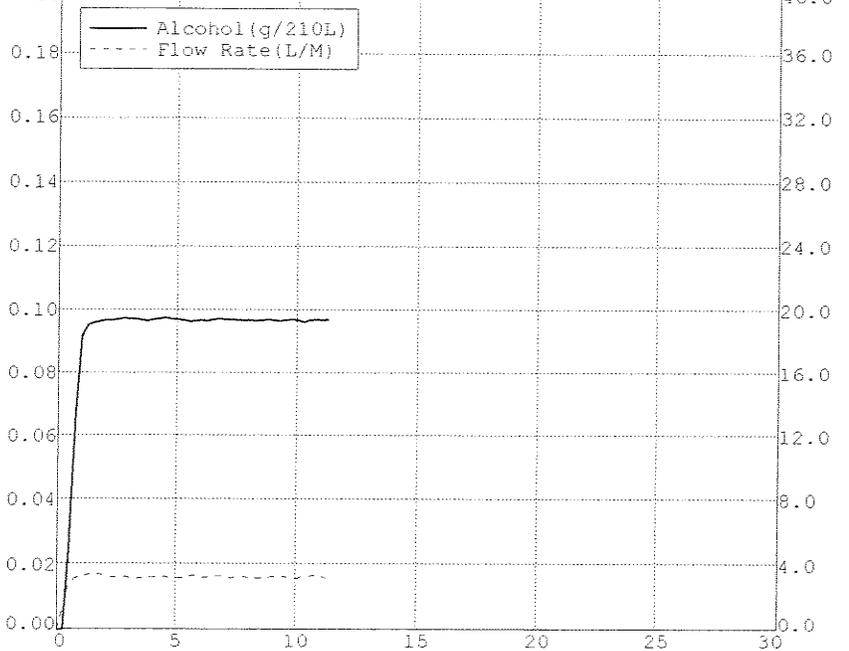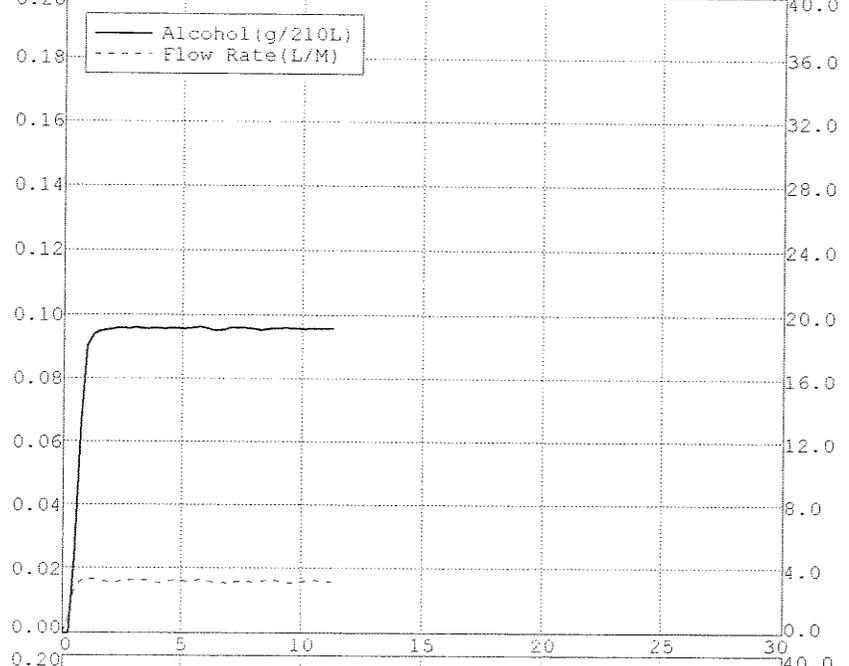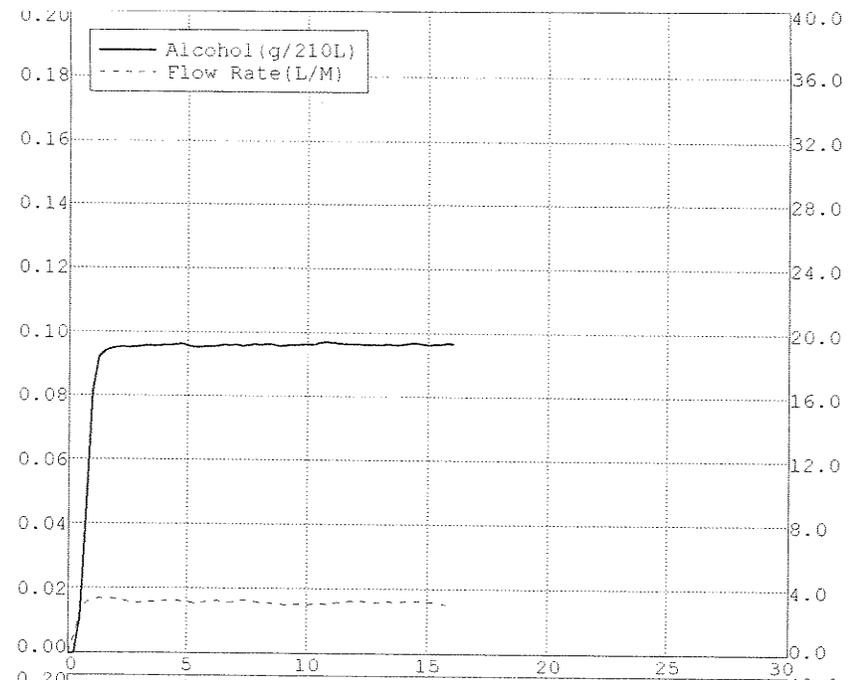

SES *RJ Bartlett* WESO #112

03-15-17