

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 03/21/2017

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 16380

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:25
INTERNAL STANDARD	VERIFIED	03:25
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	03:25
BLANK TEST	0.00	03:26
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:26
BLANK TEST	0.00	03:27
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:27
BLANK TEST	0.00	03:28

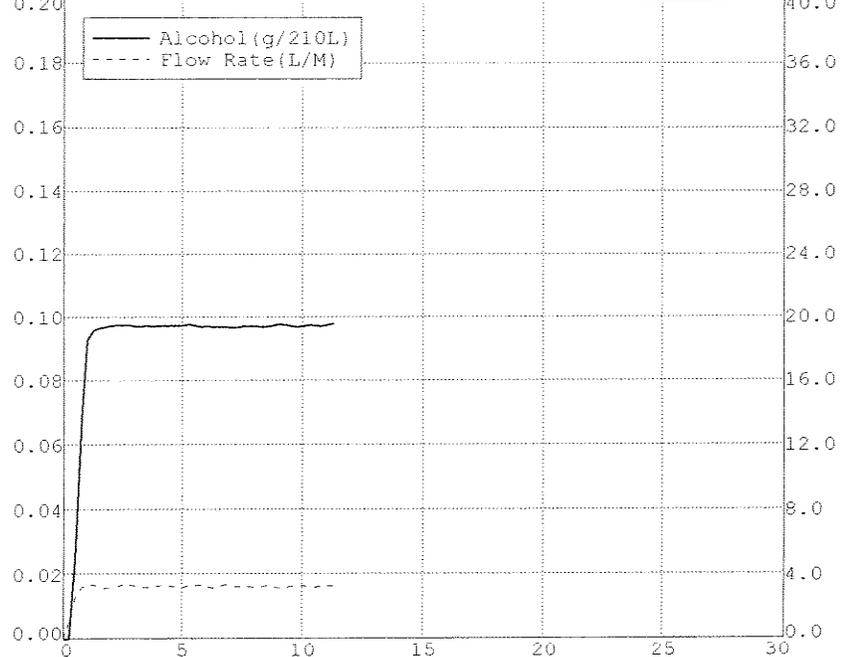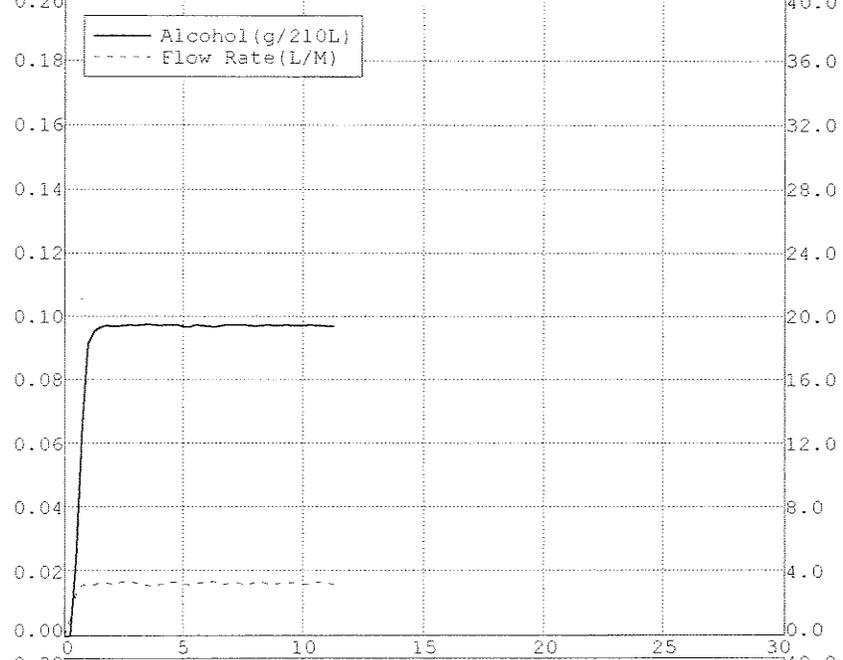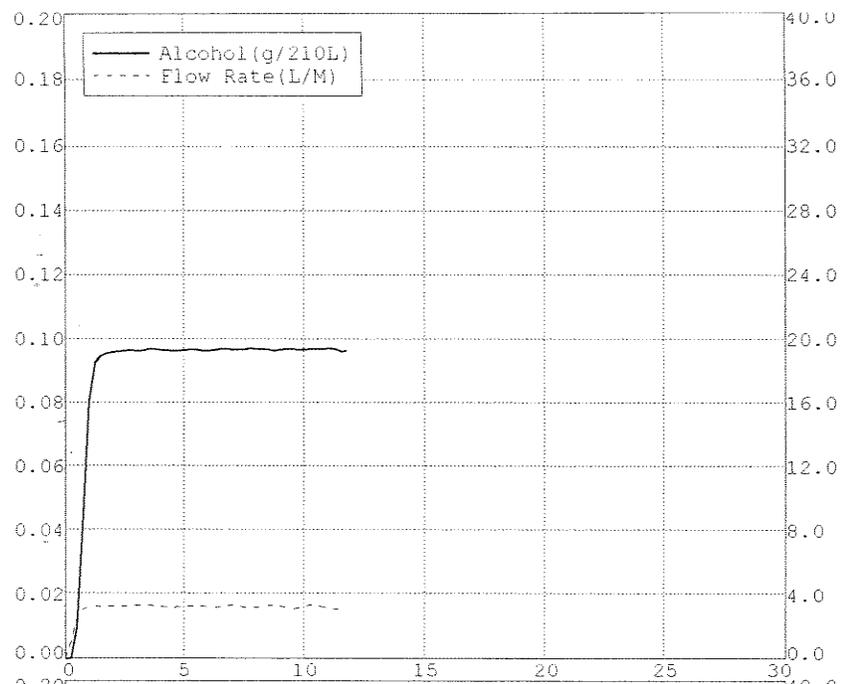

SIS RJB, Bartlett WCSO #162
 03-21-17