

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 03/27/2017

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 16380

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:14
INTERNAL STANDARD	VERIFIED	00:14
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:14
BLANK TEST	0.00	00:15
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:15
BLANK TEST	0.00	00:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:17
BLANK TEST	0.00	00:18

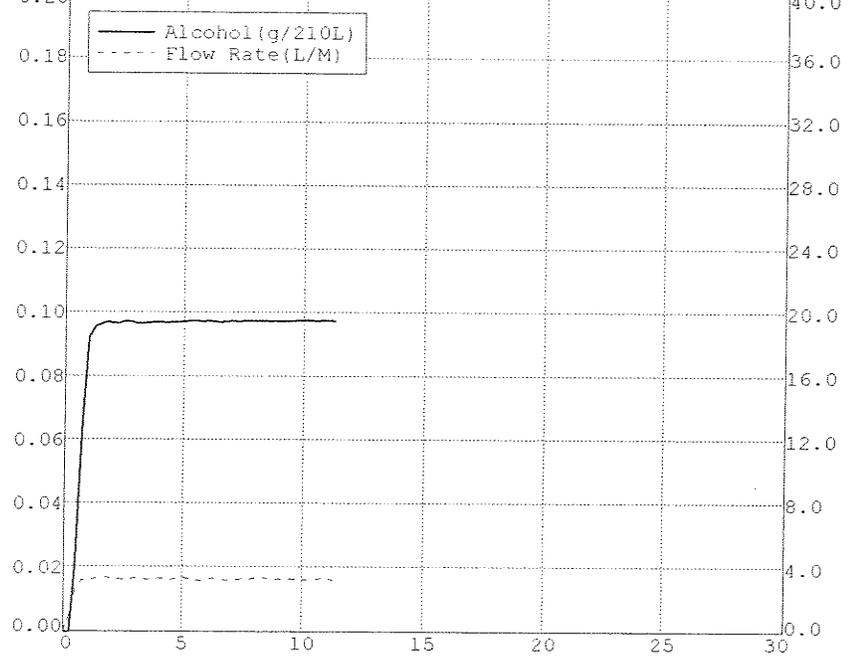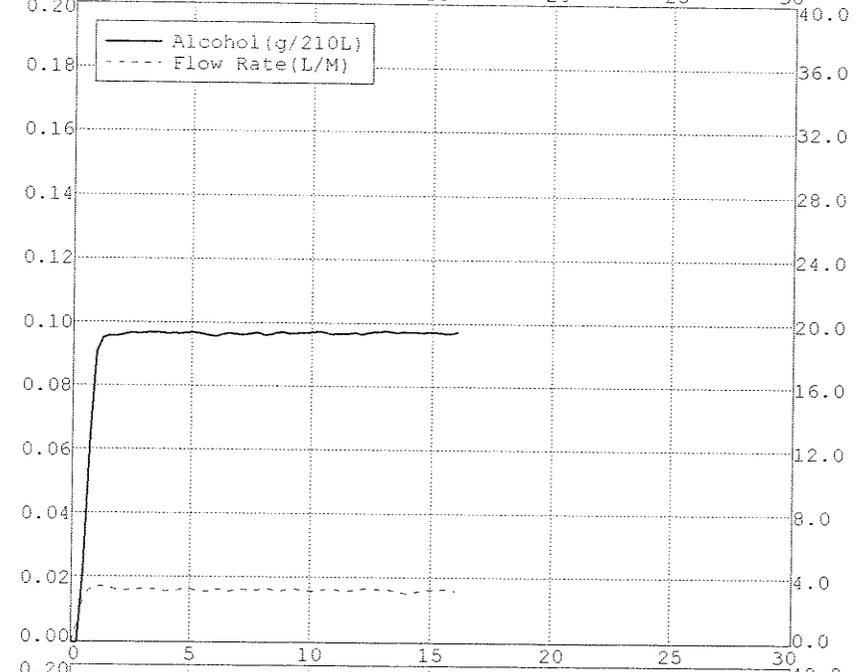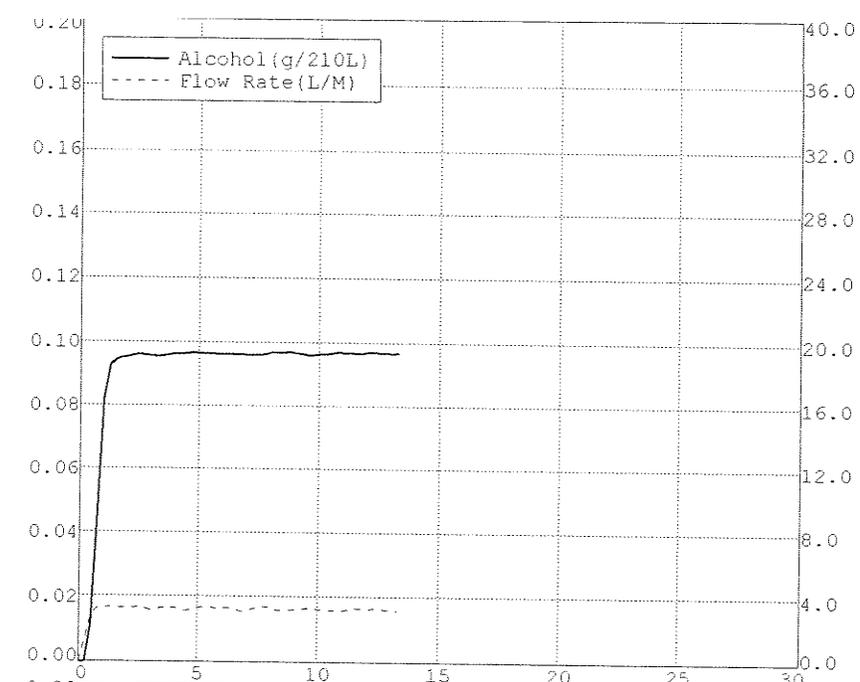

SIC Rly P... wes0#162
 03-27-17