

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/22/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:22
INTERNAL STANDARD	VERIFIED	06:22
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	06:23
BLANK TEST	0.00	06:24
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	06:24
BLANK TEST	0.00	06:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	06:25
BLANK TEST	0.00	06:26

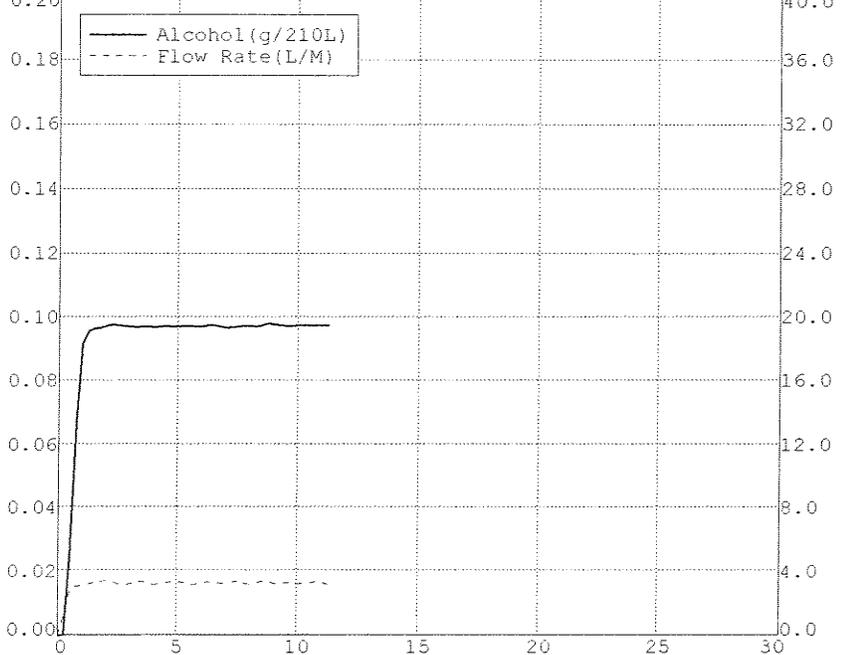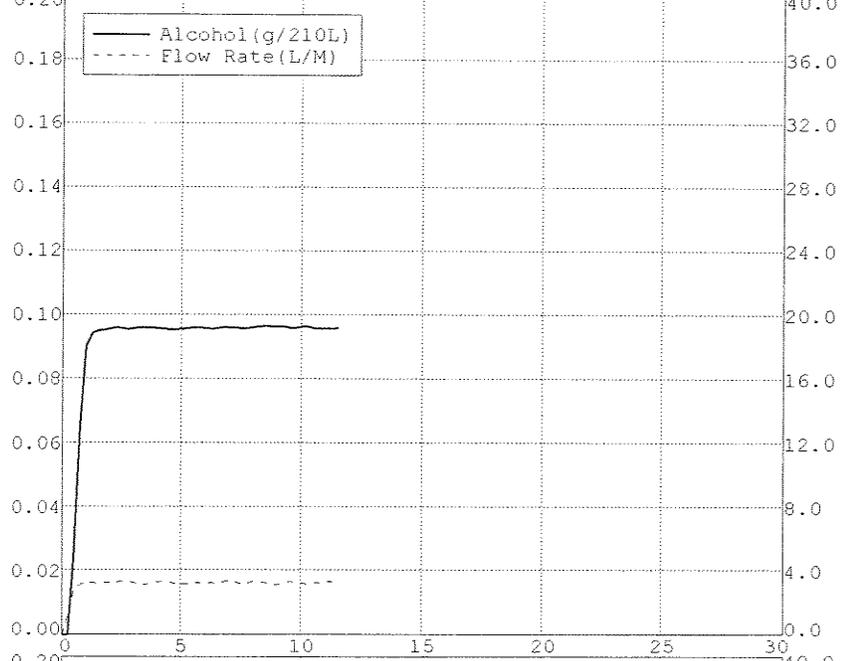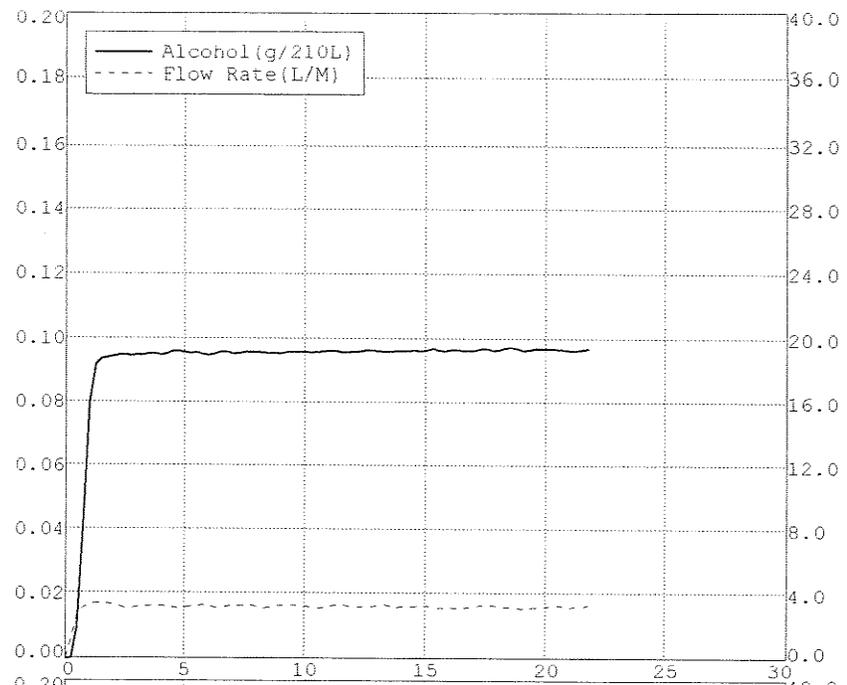

Sp. M. S. Q. #211