

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/28/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:29
INTERNAL STANDARD	VERIFIED	03:30
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	03:30
BLANK TEST	0.00	03:31
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:31
BLANK TEST	0.00	03:32
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	03:32
BLANK TEST	0.00	03:33

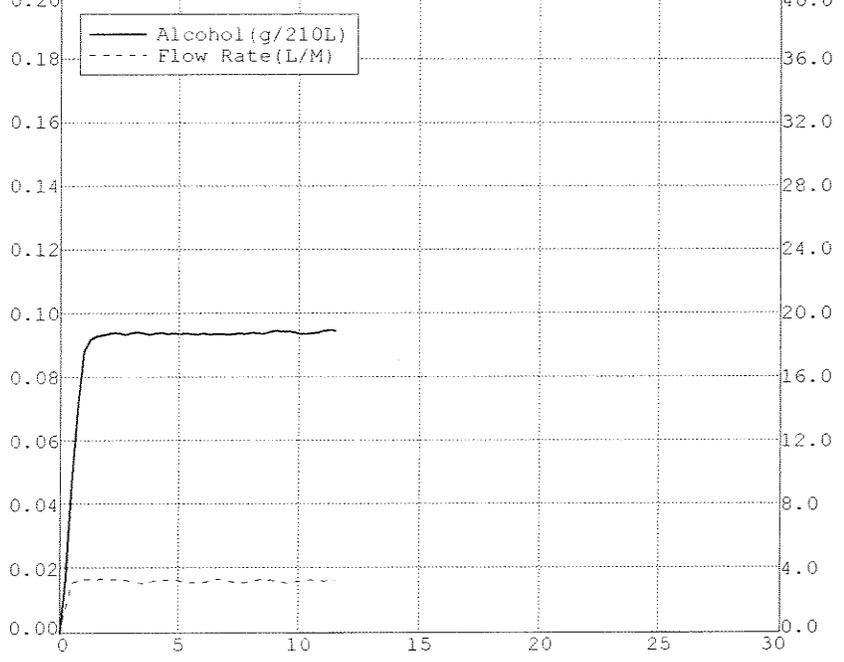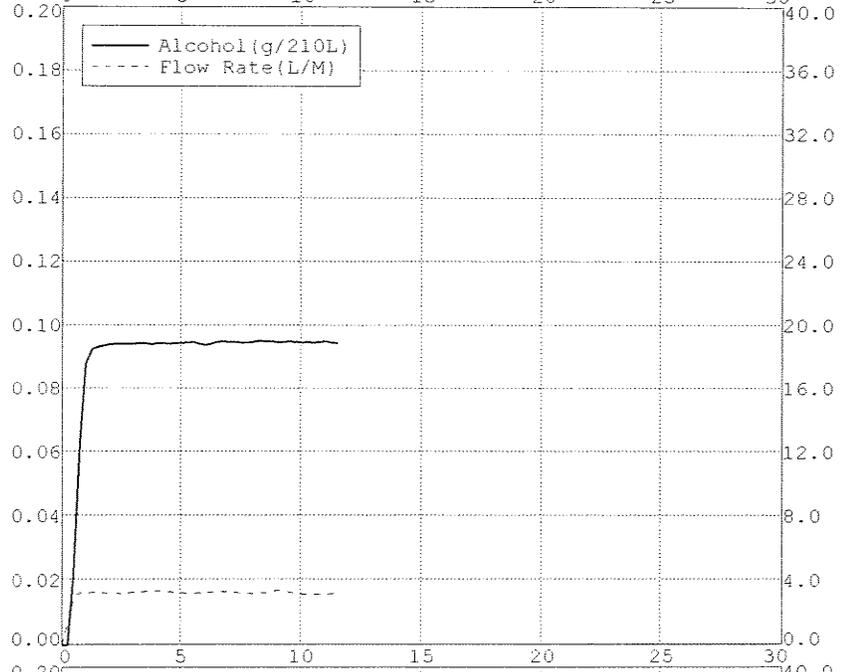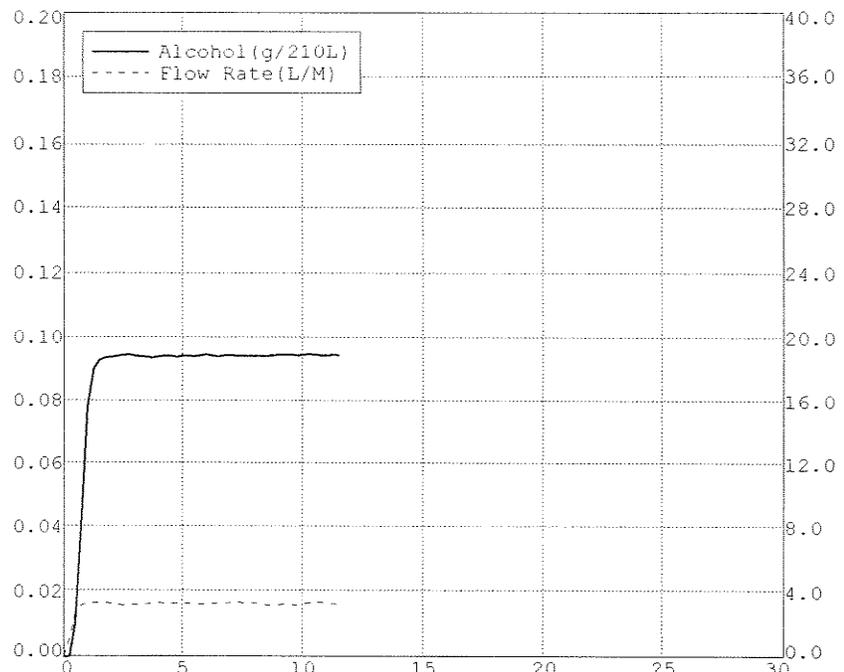

Joe M. B. [Signature] #248 4/28/17