

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 05/02/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:18
INTERNAL STANDARD	VERIFIED	04:18
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	04:18
BLANK TEST	0.00	04:19
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	04:20
BLANK TEST	0.00	04:21
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	04:21
BLANK TEST	0.00	04:22

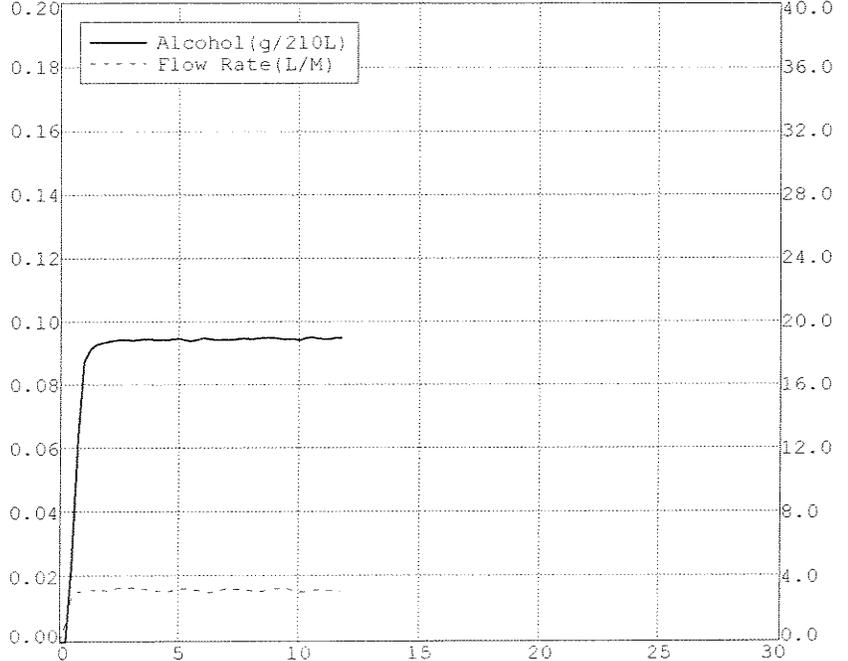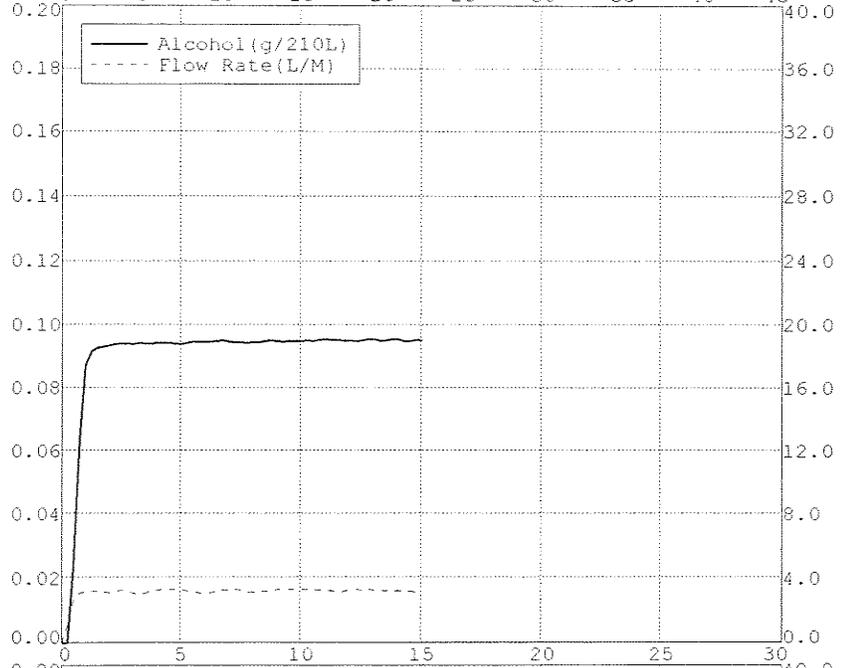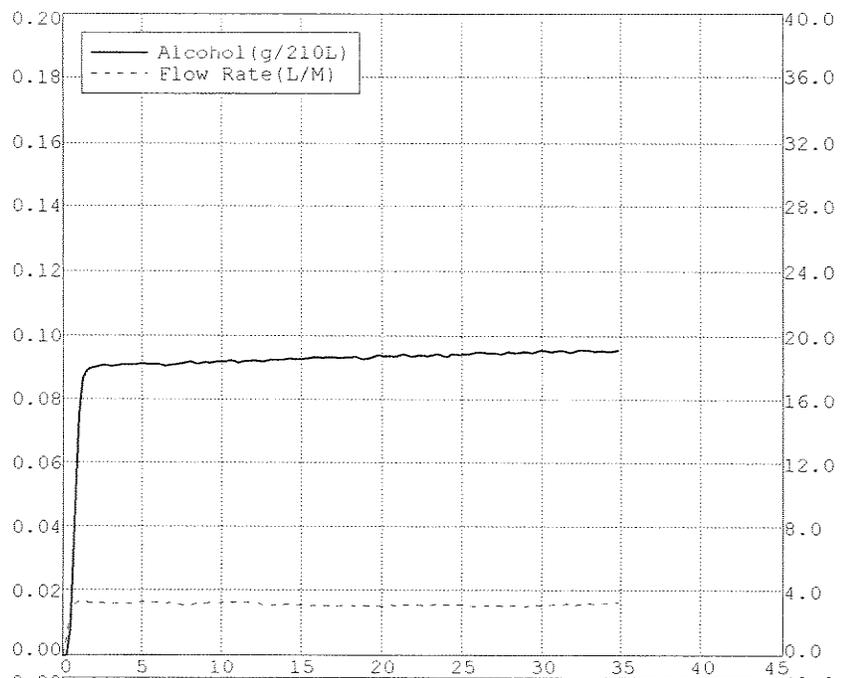

*Charles B. Geisler #241*