

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/11/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:51
INTERNAL STANDARD	VERIFIED	02:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:52
BLANK TEST	0.00	02:53
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:53
BLANK TEST	0.00	02:54
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:54
BLANK TEST	0.00	02:55

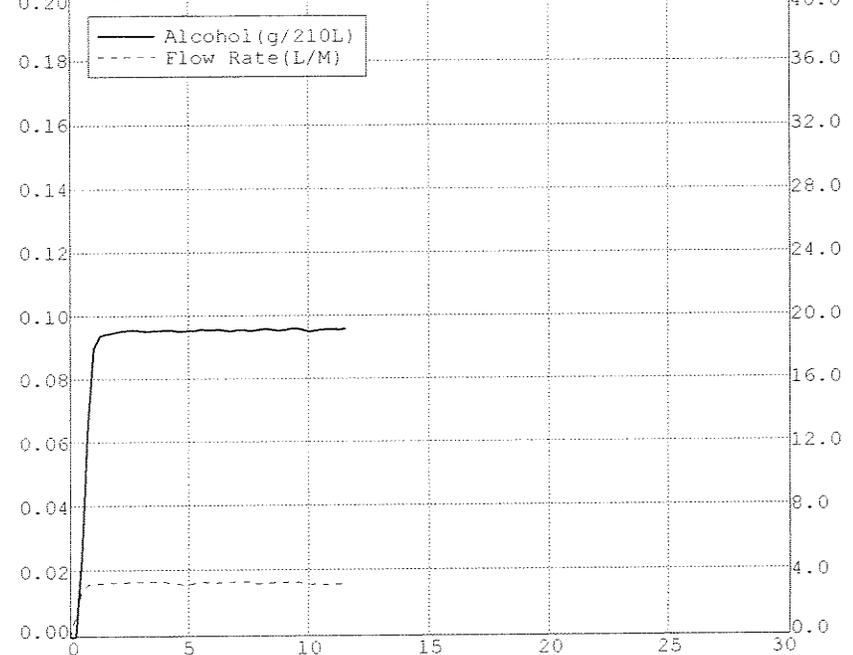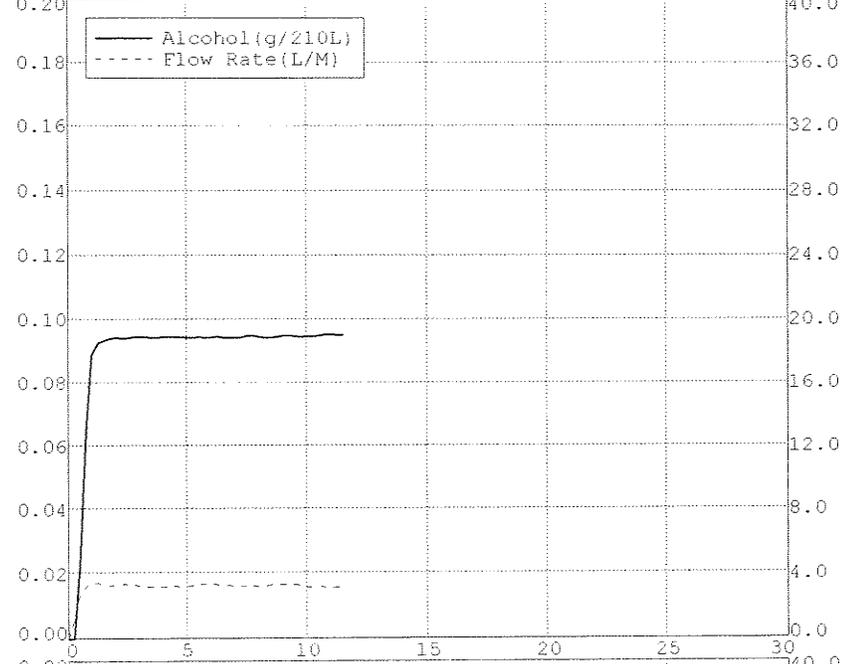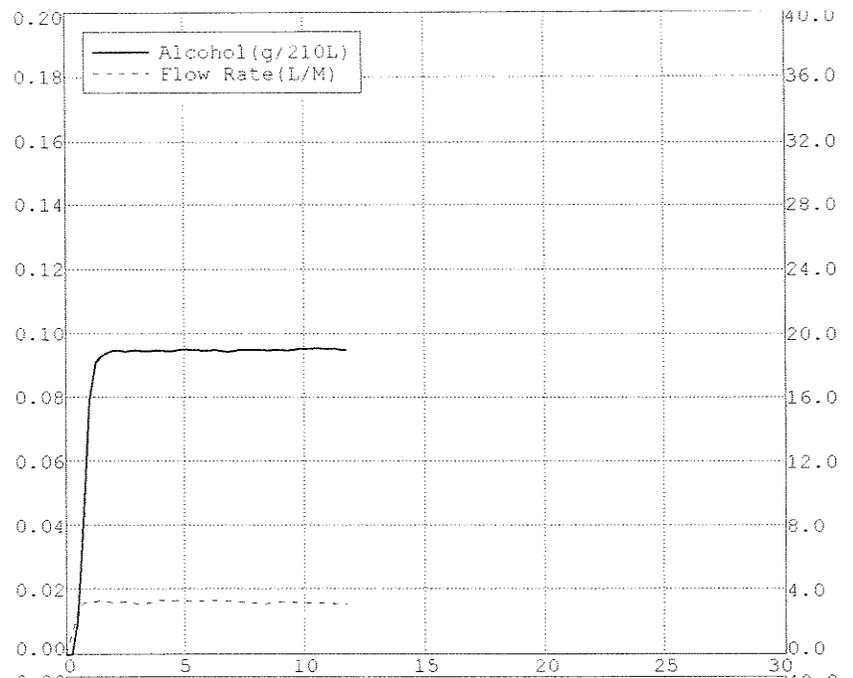

Charles B. Geisler #2116