

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/15/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:43
INTERNAL STANDARD	VERIFIED	10:43
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	10:43
BLANK TEST	0.00	10:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:44
BLANK TEST	0.00	10:45
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:46
BLANK TEST	0.00	10:47

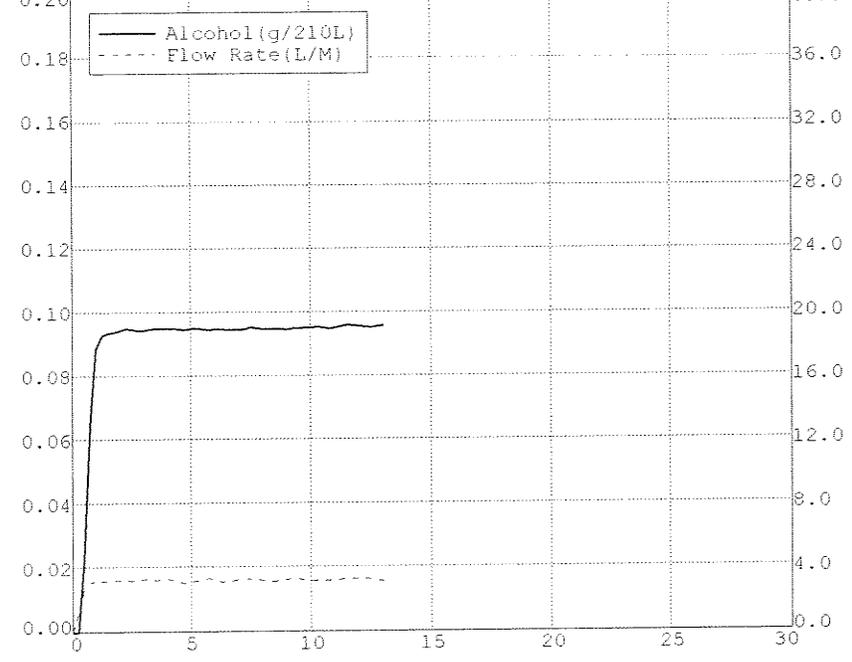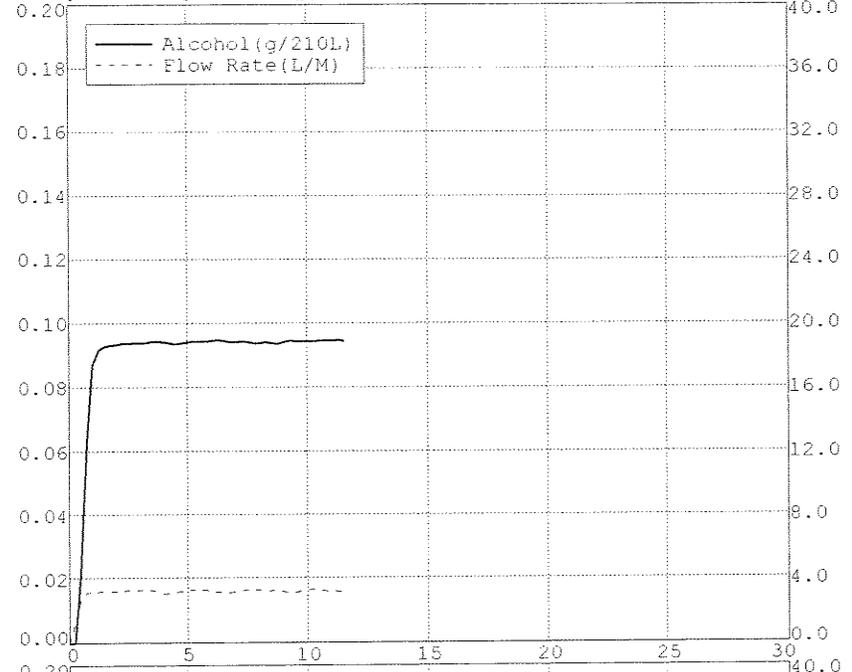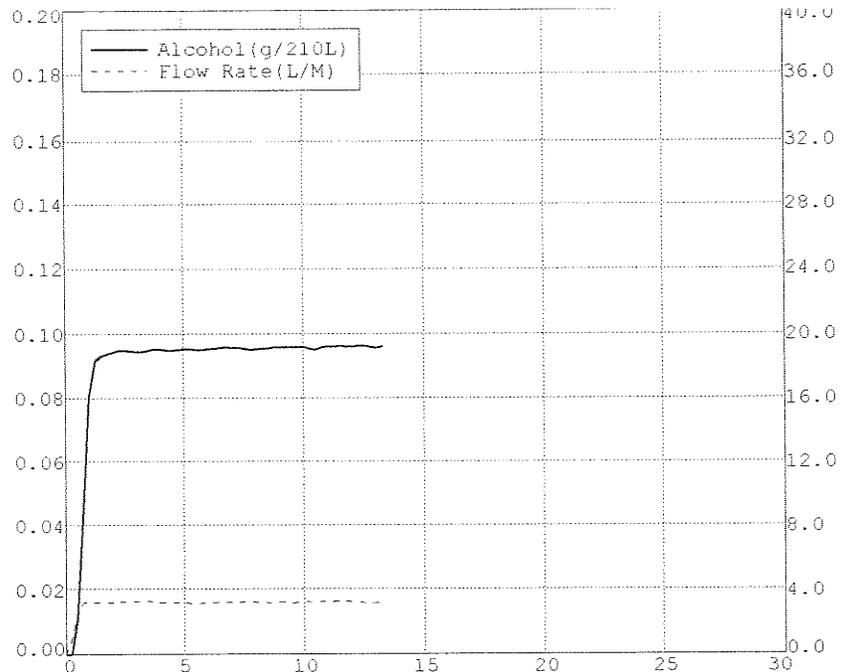

Sp. Ch. S. D. 5/15/17