

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 06/03/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:36
INTERNAL STANDARD	VERIFIED	04:37
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	04:37
BLANK TEST	0.00	04:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:38
BLANK TEST	0.00	04:39
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	04:39
BLANK TEST	0.00	04:40

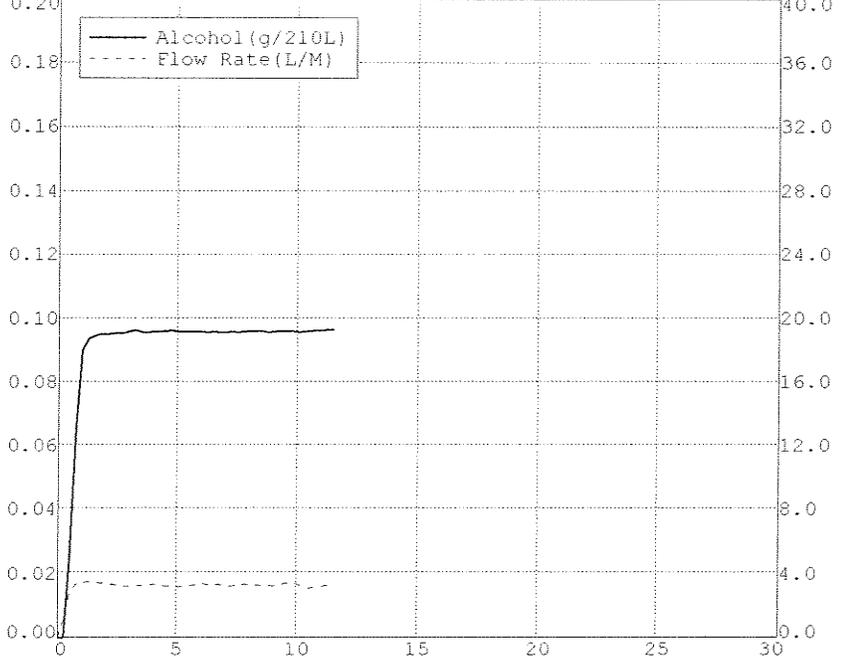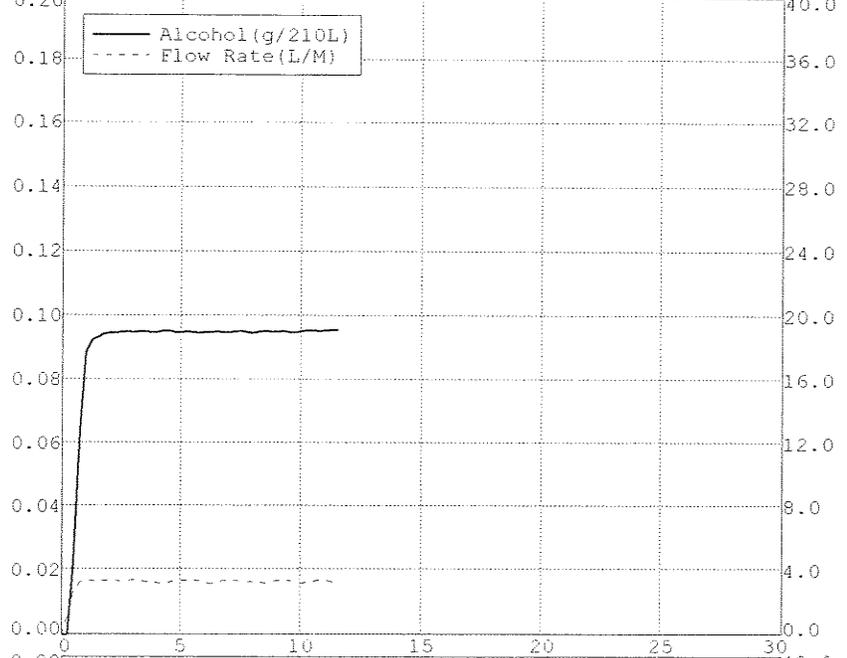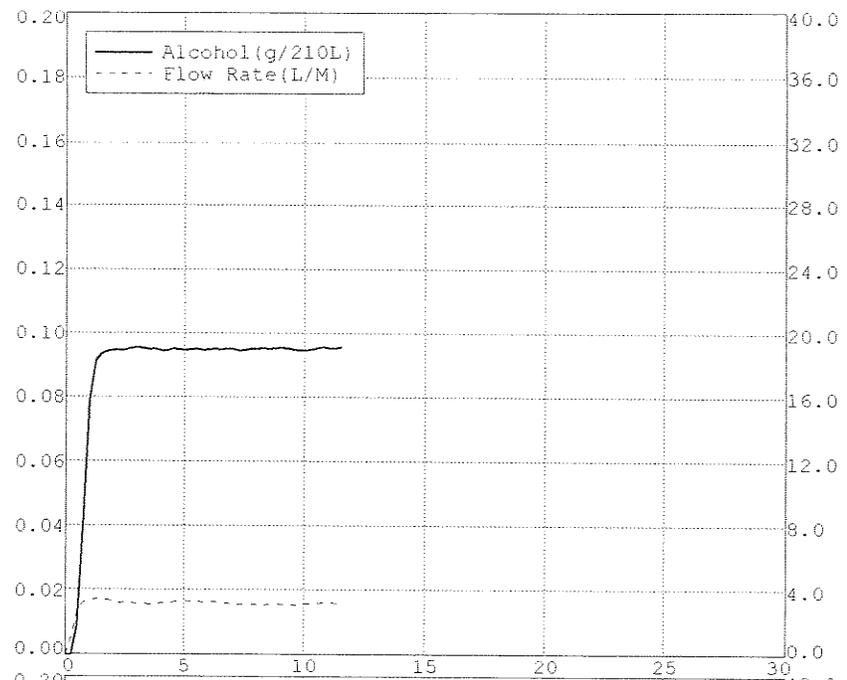

*Charles B. Geisler* #248