

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 06/09/2017

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:34
INTERNAL STANDARD	VERIFIED	21:35
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	21:35
BLANK TEST	0.00	21:36
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	21:36
BLANK TEST	0.00	21:37
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:37
BLANK TEST	0.00	21:38

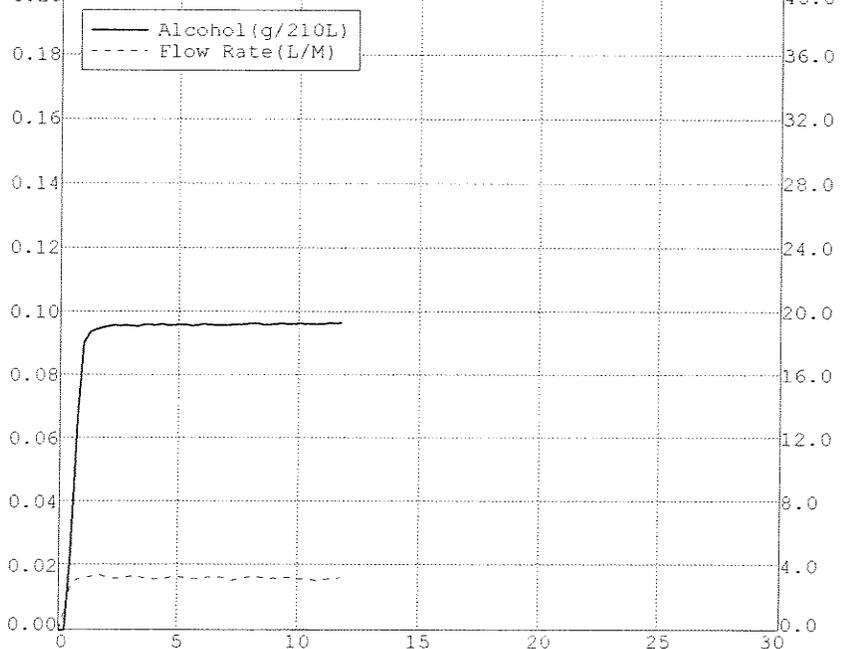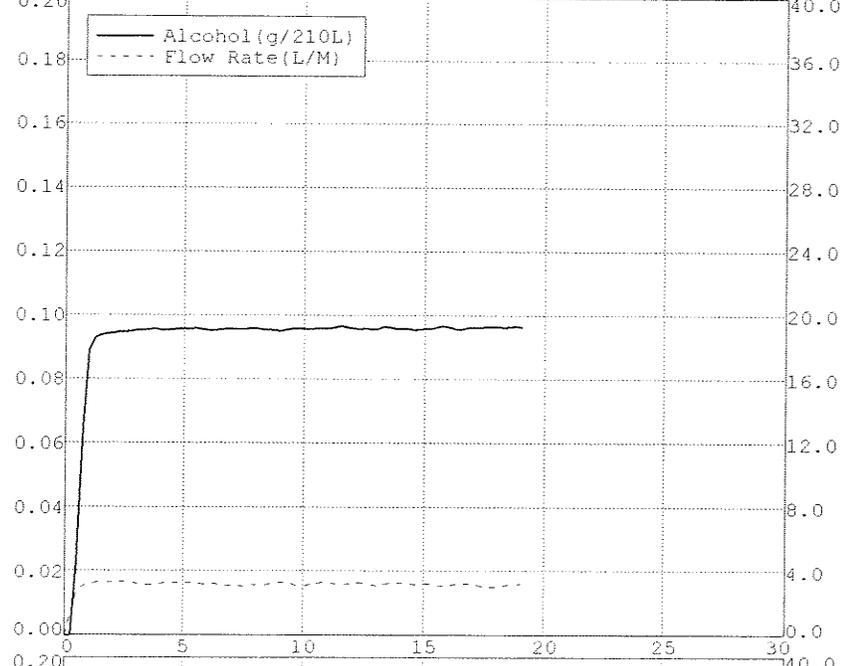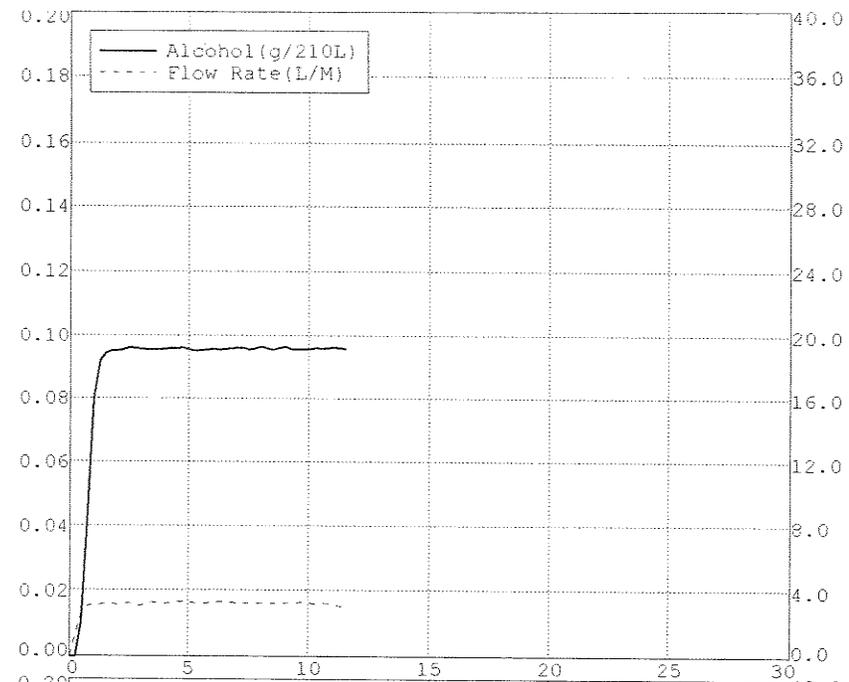

*Signature* #246