

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 06/17/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:59
INTERNAL STANDARD	VERIFIED	03:59
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	03:59
BLANK TEST	0.00	04:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:00
BLANK TEST	0.00	04:01
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	04:02
BLANK TEST	0.00	04:02

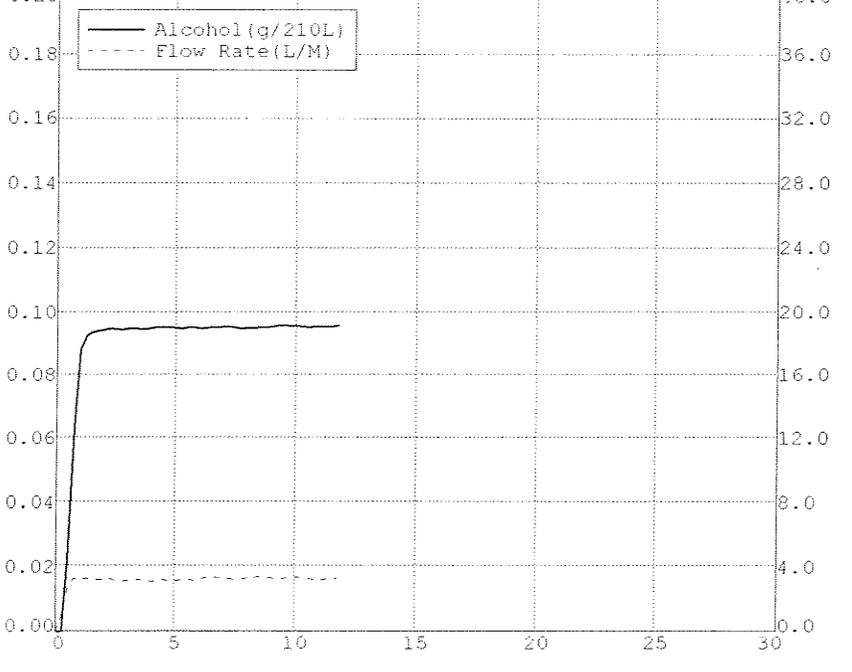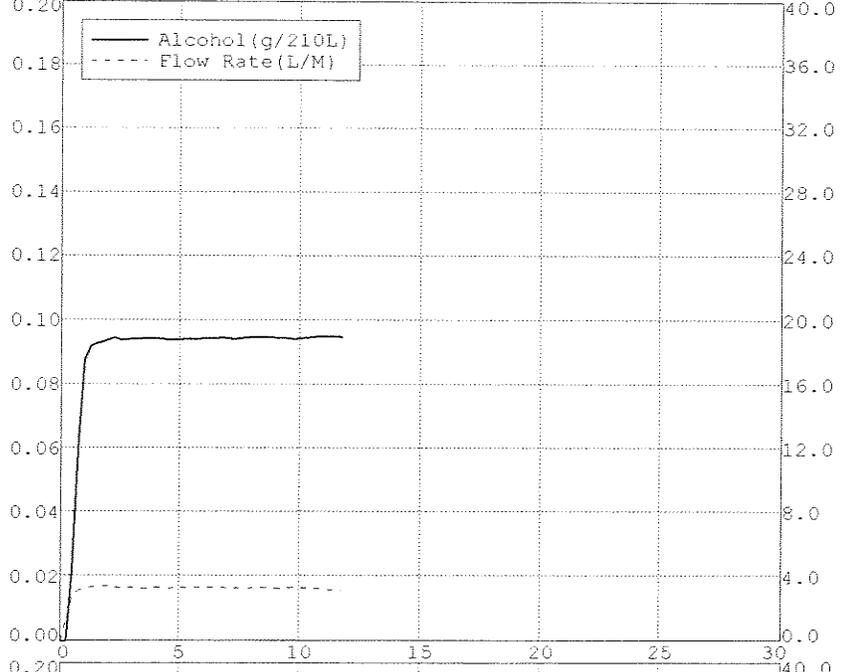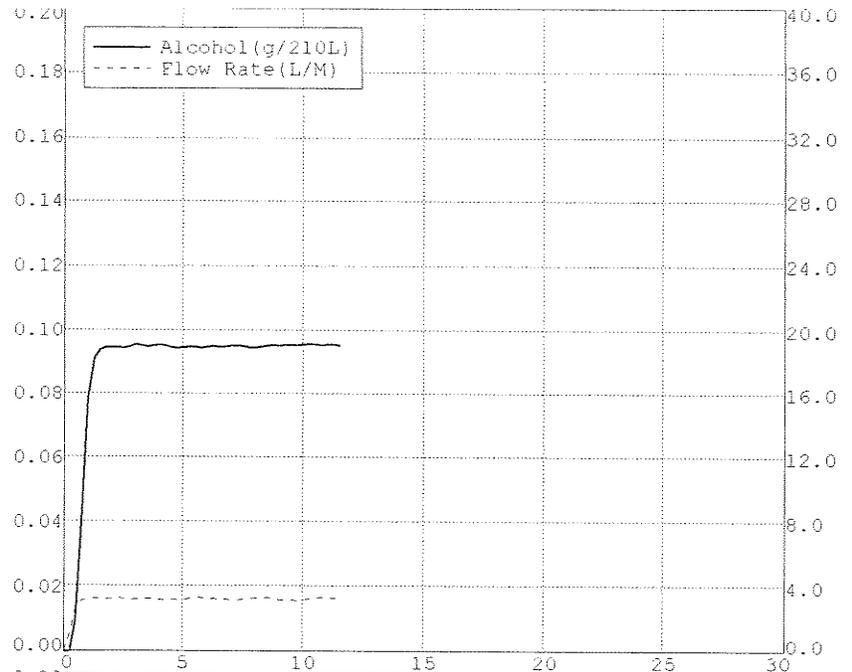

Sgt. Charles B. Geisler #241