

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 07/02/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:23
INTERNAL STANDARD	VERIFIED	01:23
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:23
BLANK TEST	0.00	01:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:24
BLANK TEST	0.00	01:25
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:26
BLANK TEST	0.00	01:27

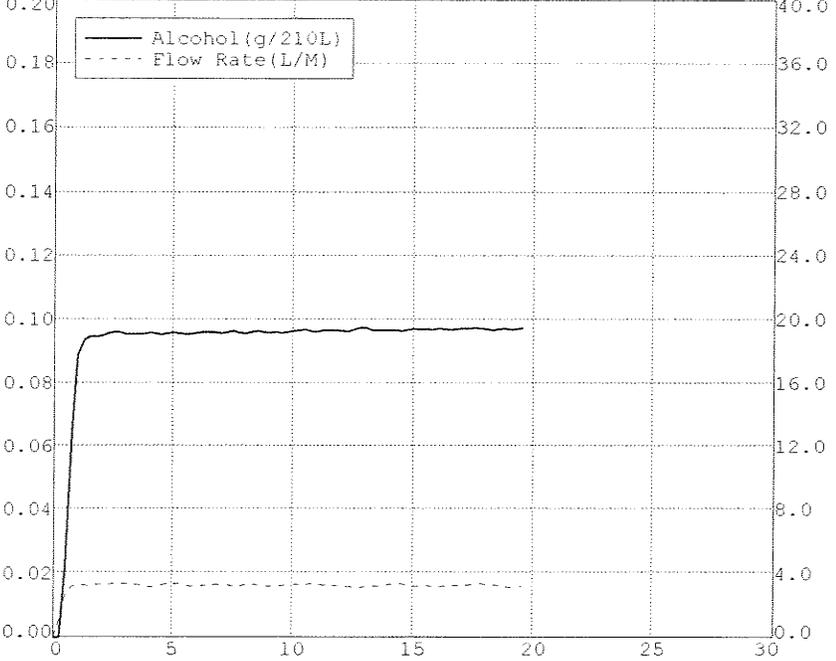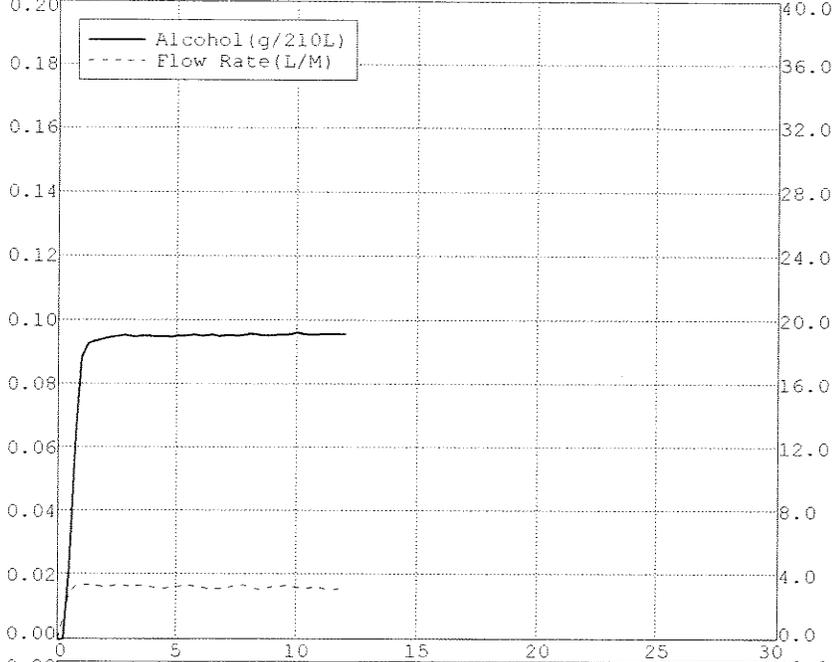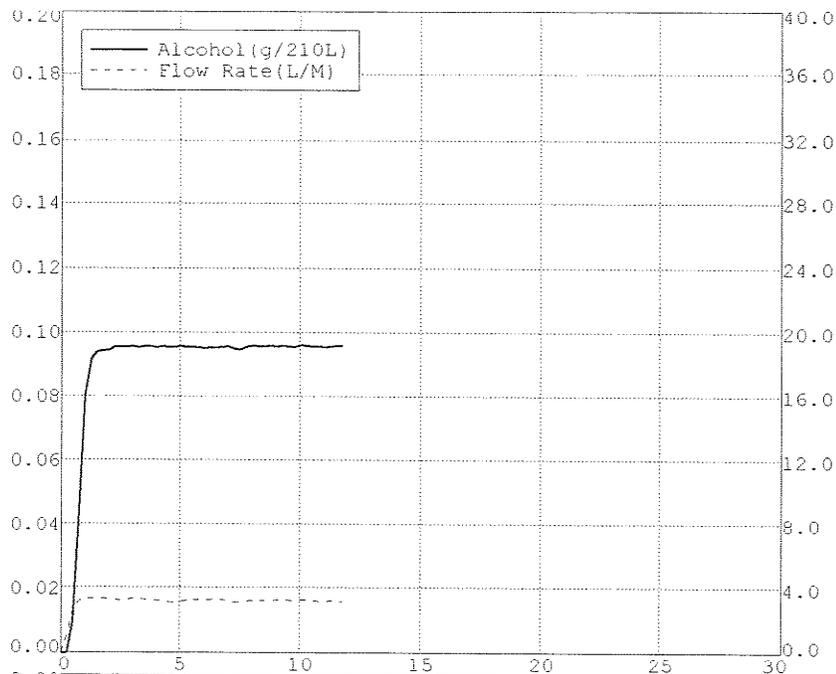

Charles B. Geisler #2418