

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 07/10/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:44
INTERNAL STANDARD	VERIFIED	19:44
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	19:44
BLANK TEST	0.00	19:45
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	19:46
BLANK TEST	0.00	19:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	19:47
BLANK TEST	0.00	19:48

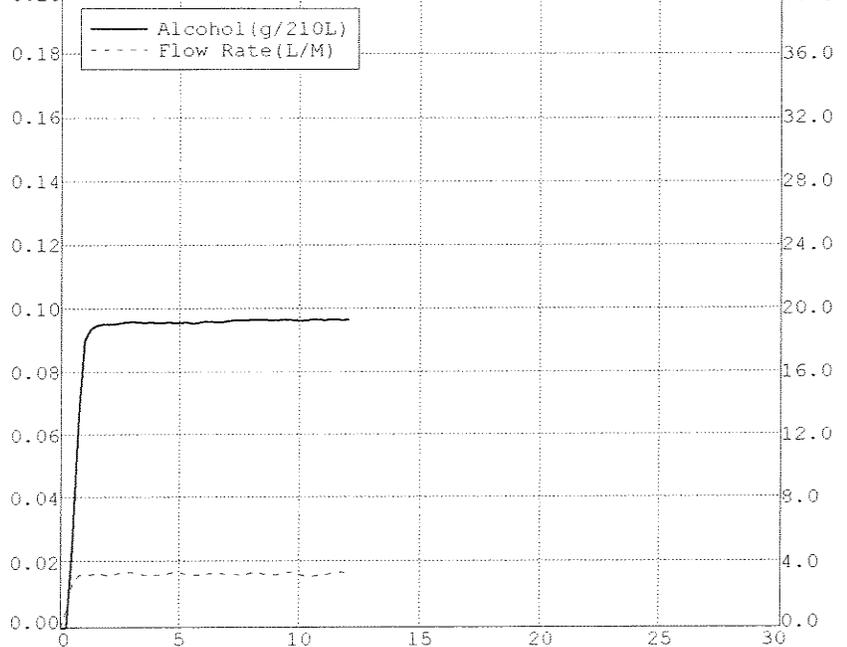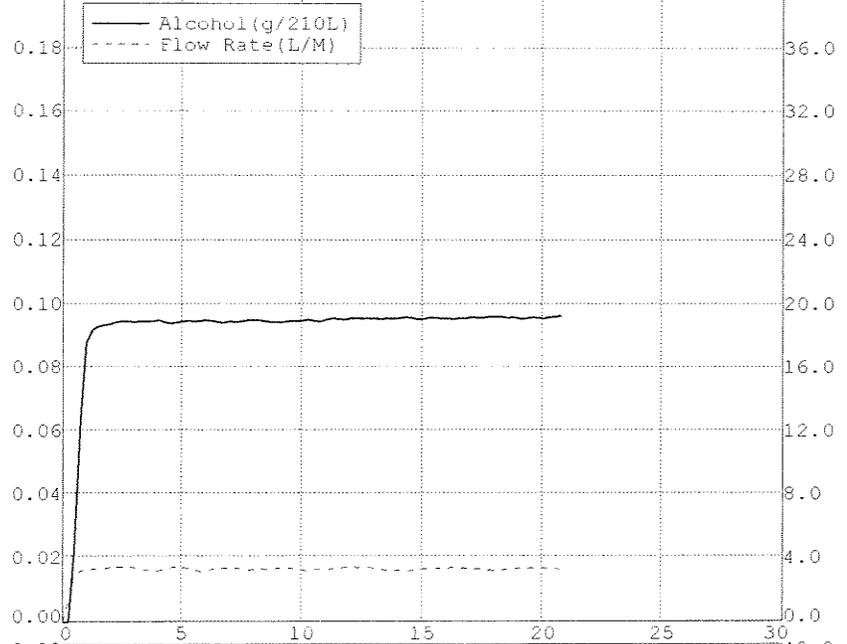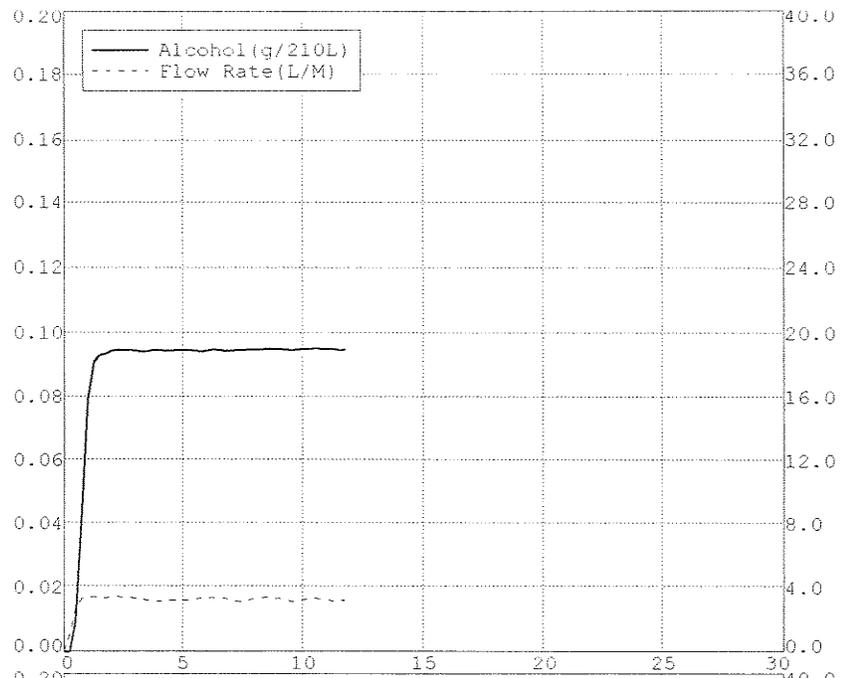

Signature
#248