

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 07/17/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:02
INTERNAL STANDARD	VERIFIED	02:02
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	02:03
BLANK TEST	0.00	02:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:04
BLANK TEST	0.00	02:05
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	02:05
BLANK TEST	0.00	02:06

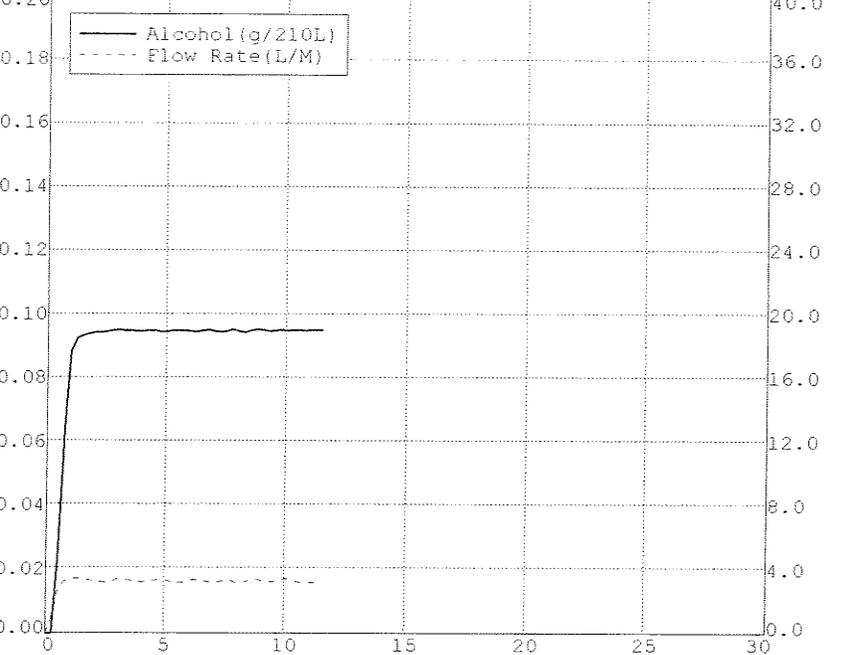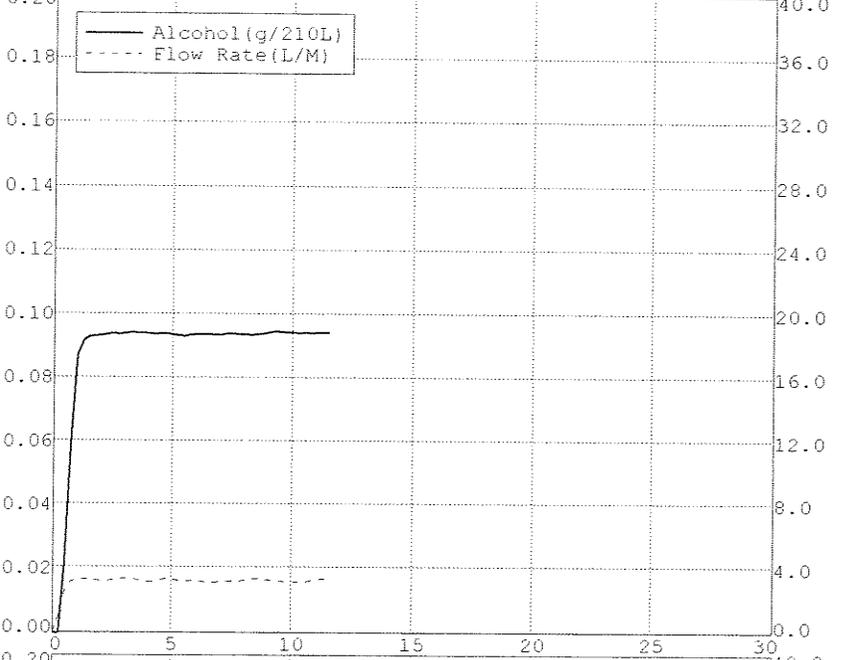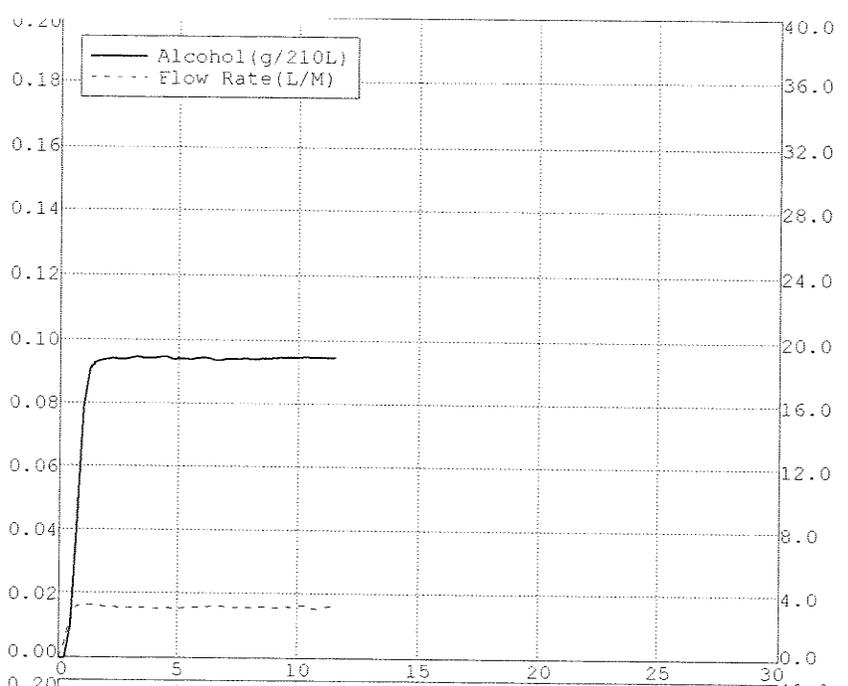

By Chl B. Ld #248