

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 07/25/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:57
INTERNAL STANDARD	VERIFIED	05:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	05:57
BLANK TEST	0.00	05:58
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	05:58
BLANK TEST	0.00	05:59
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	06:00
BLANK TEST	0.00	06:01

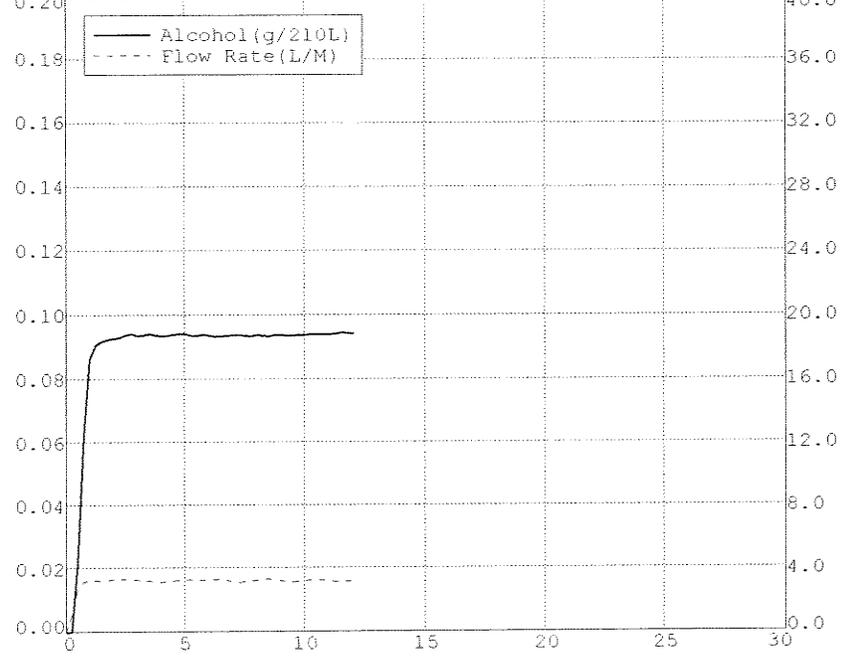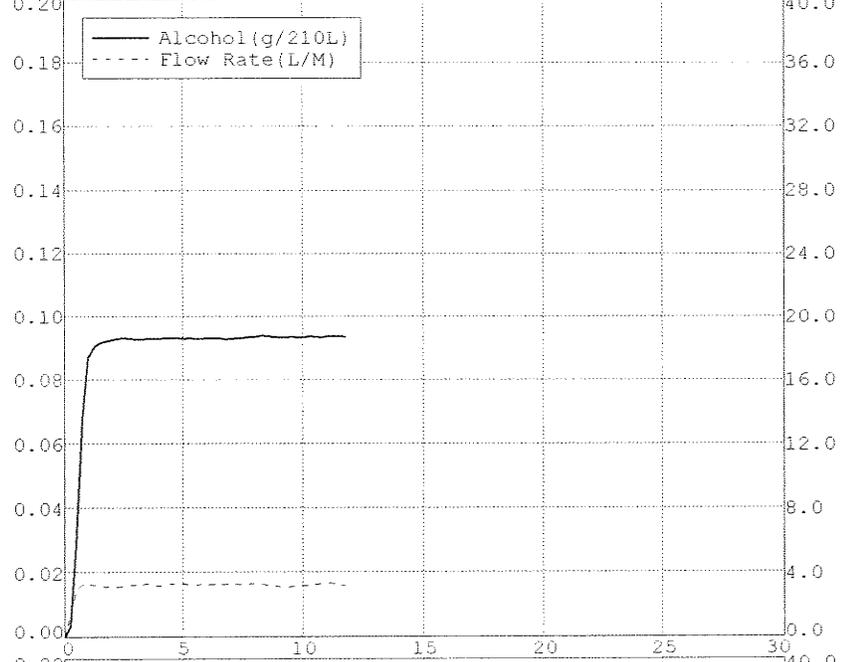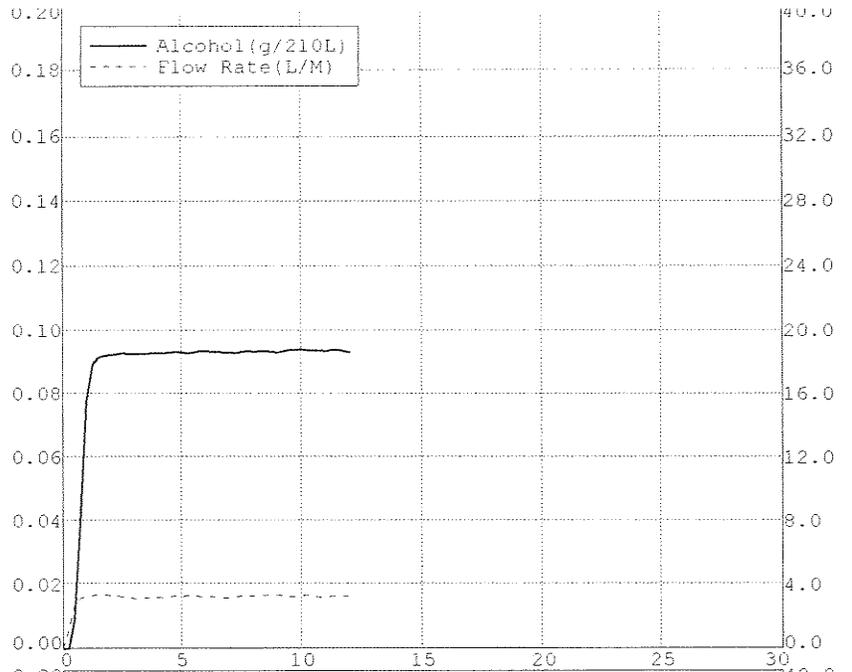

*Charles B. Geisler* #241