

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 07/30/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:55
INTERNAL STANDARD	VERIFIED	02:55
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	02:55
BLANK TEST	0.00	02:56
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:56
BLANK TEST	0.00	02:57
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:57
BLANK TEST	0.00	02:58

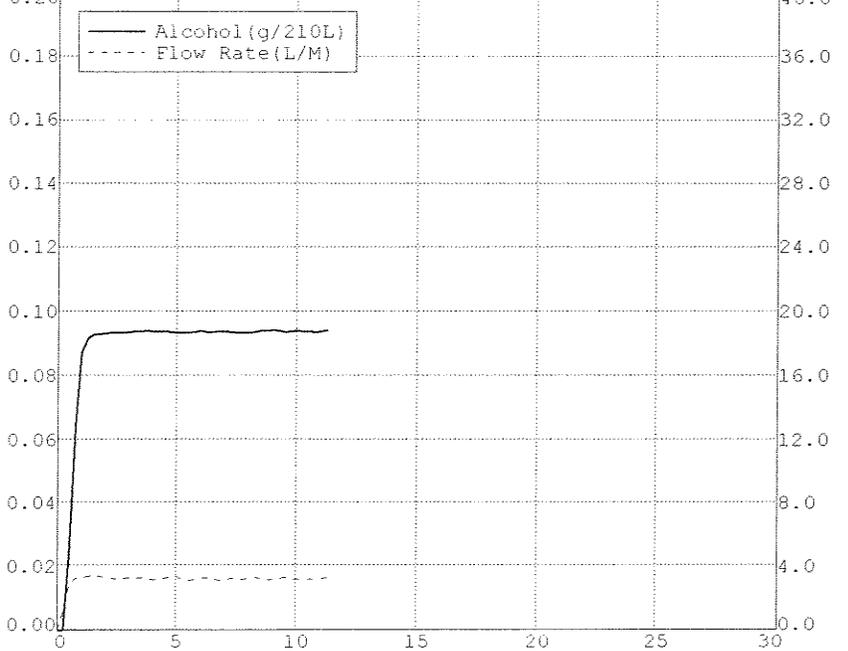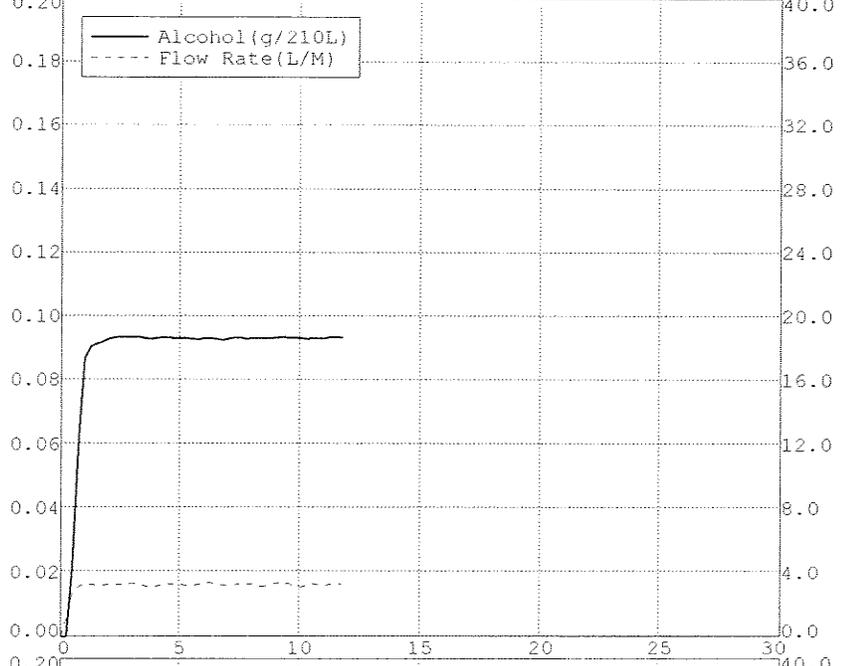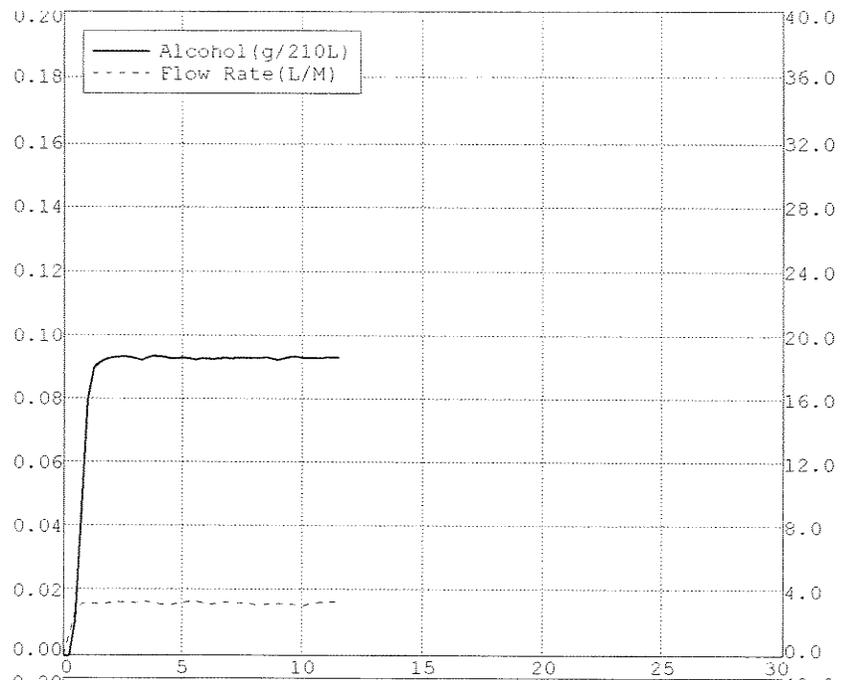

*Sgt. Ch. B. Geisler #241*