

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 08/04/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:38
INTERNAL STANDARD	VERIFIED	00:38
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	00:38
BLANK TEST	0.00	00:39
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:39
BLANK TEST	0.00	00:40
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	00:40
BLANK TEST	0.00	00:41

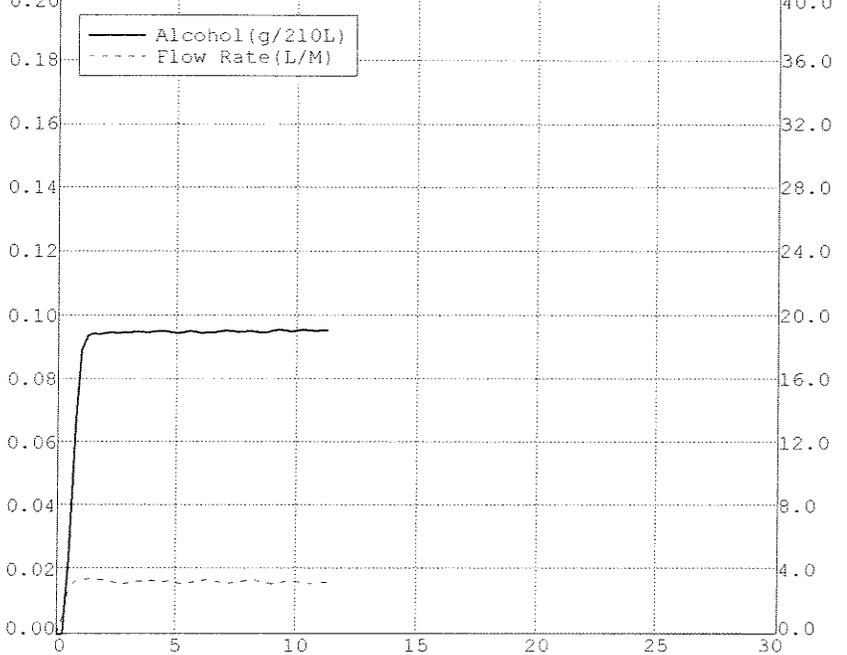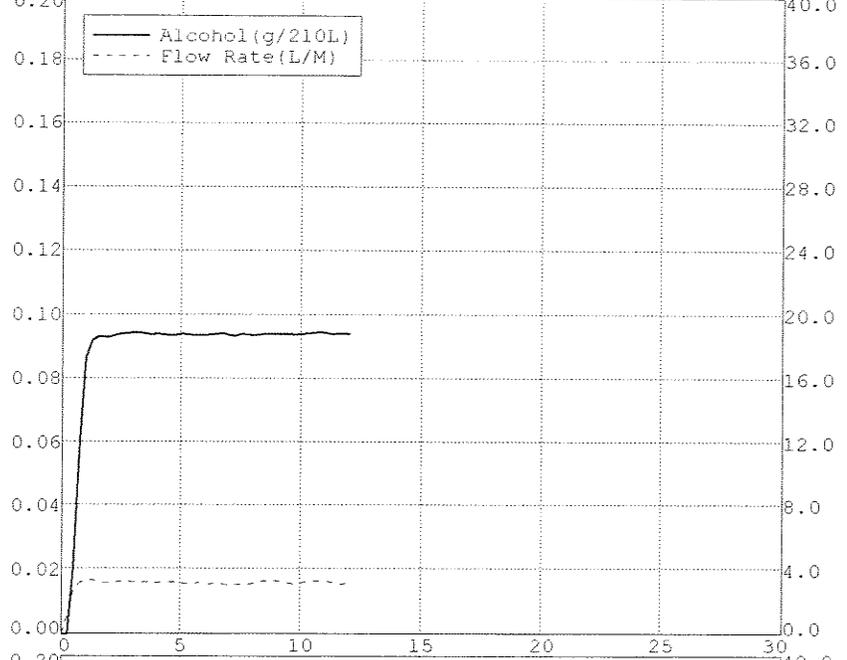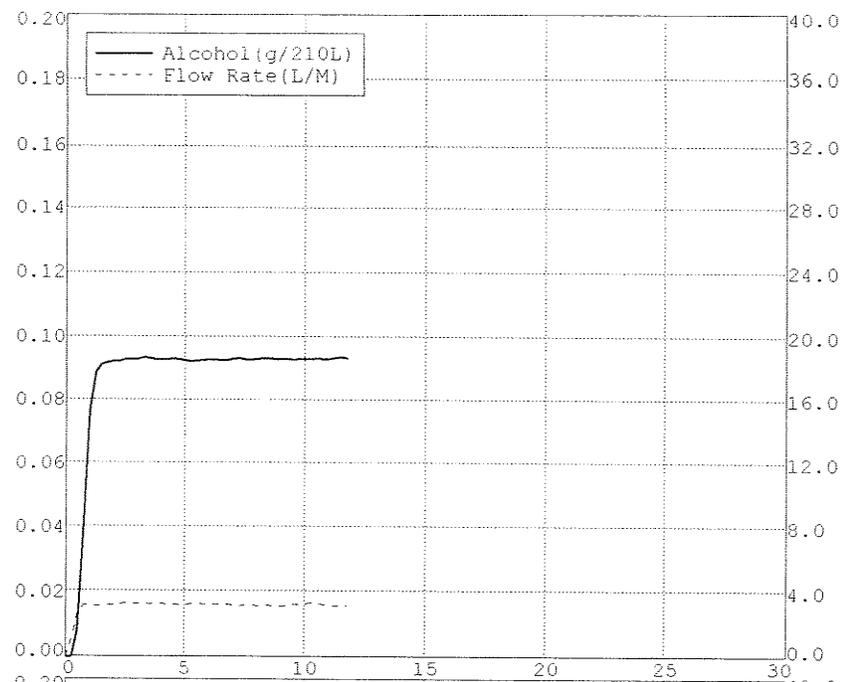

Charles B. Geisler #29