

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 08/12/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:12
INTERNAL STANDARD	VERIFIED	00:12
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	00:13
BLANK TEST	0.00	00:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:14
BLANK TEST	0.00	00:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:15
BLANK TEST	0.00	00:16

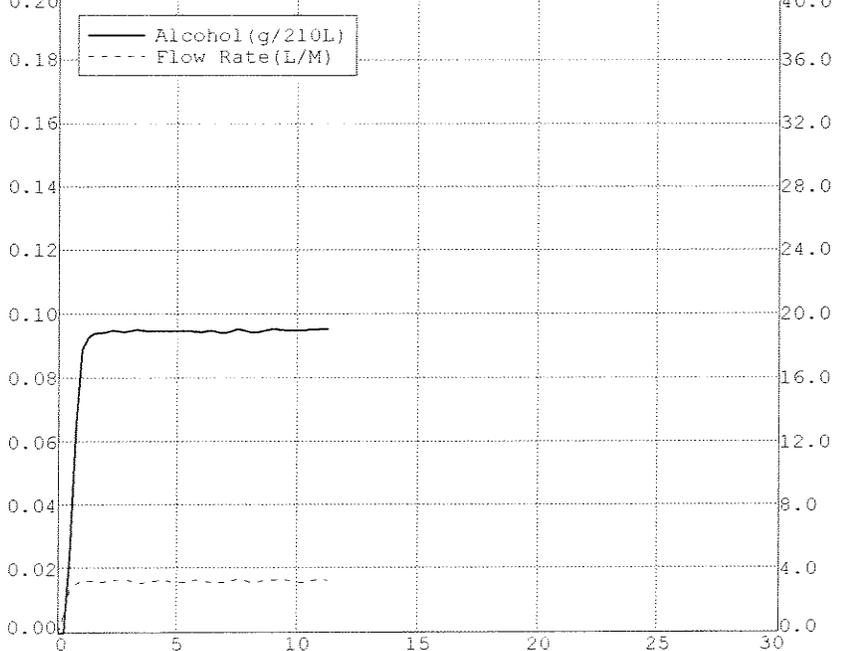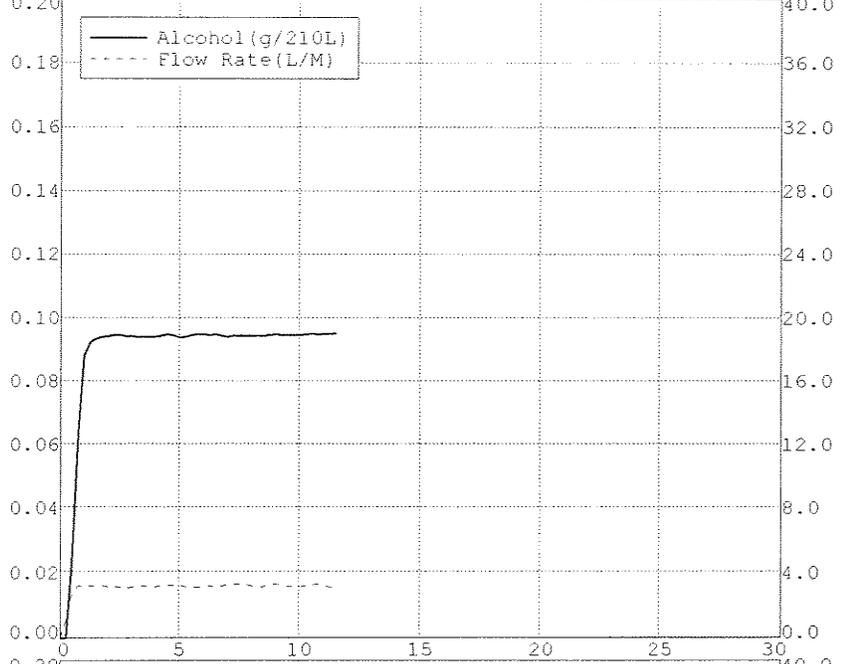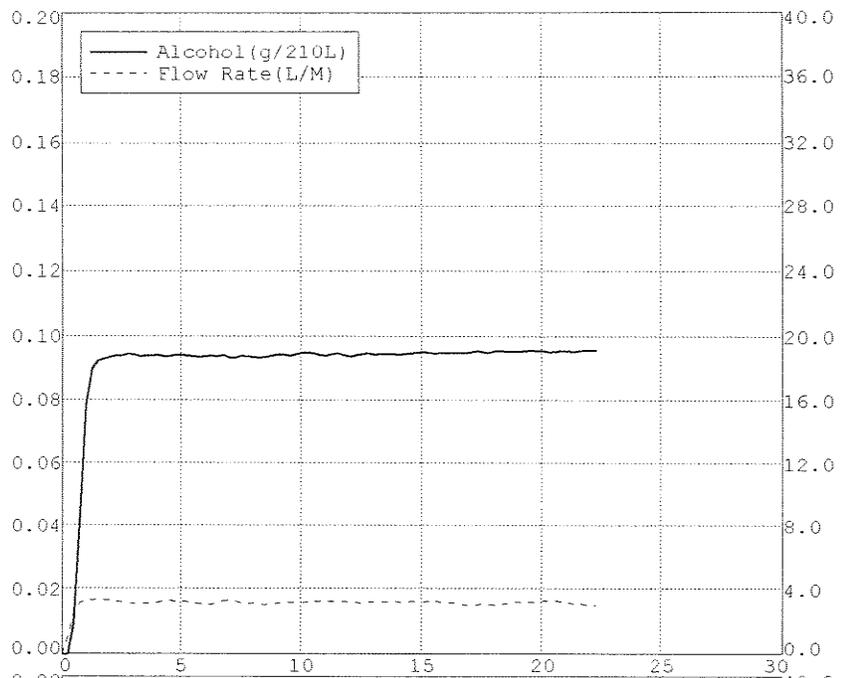

Charles B. Geisler #241