

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 08/21/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:36
INTERNAL STANDARD	VERIFIED	21:36
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	21:36
BLANK TEST	0.00	21:37
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	21:37
BLANK TEST	0.00	21:38
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	21:38
BLANK TEST	0.00	21:39

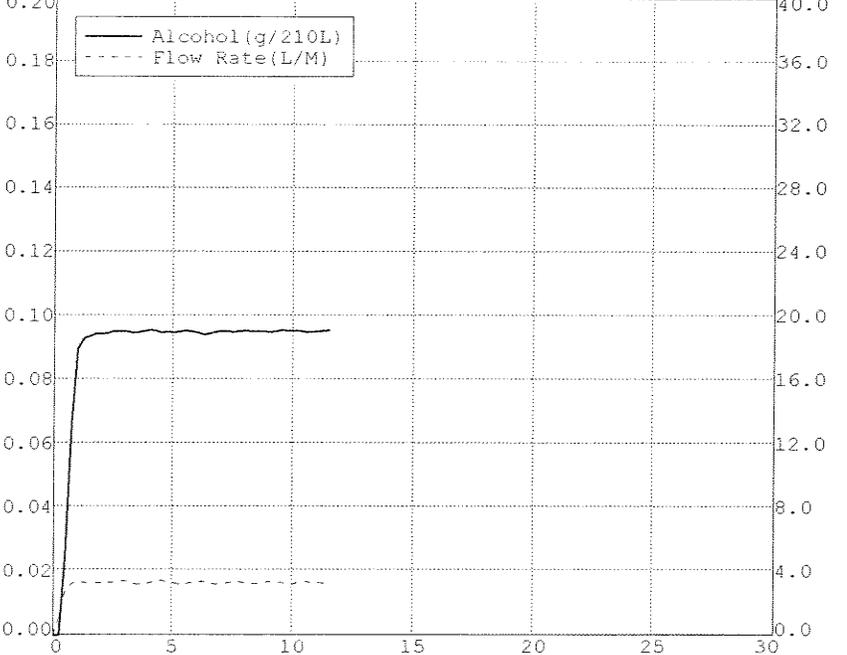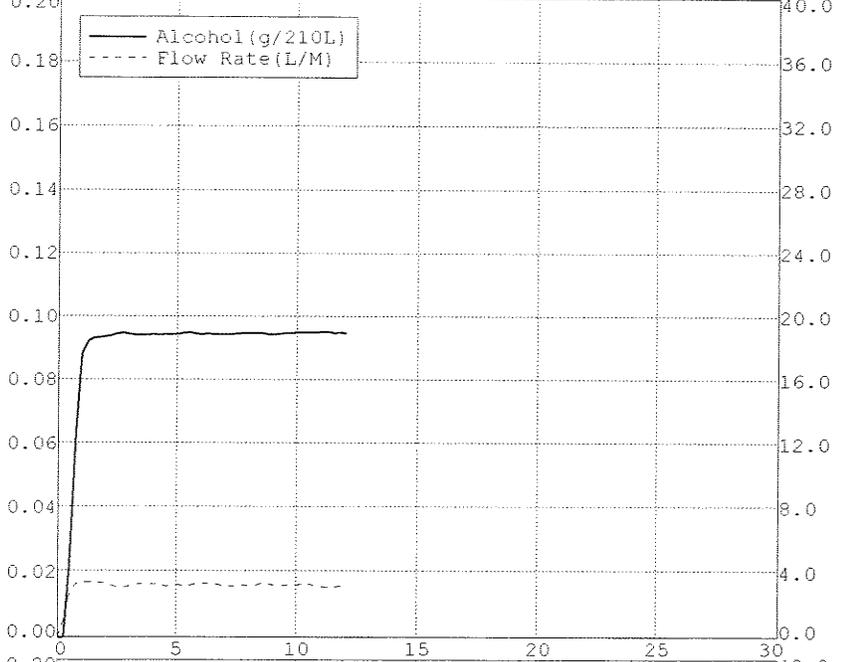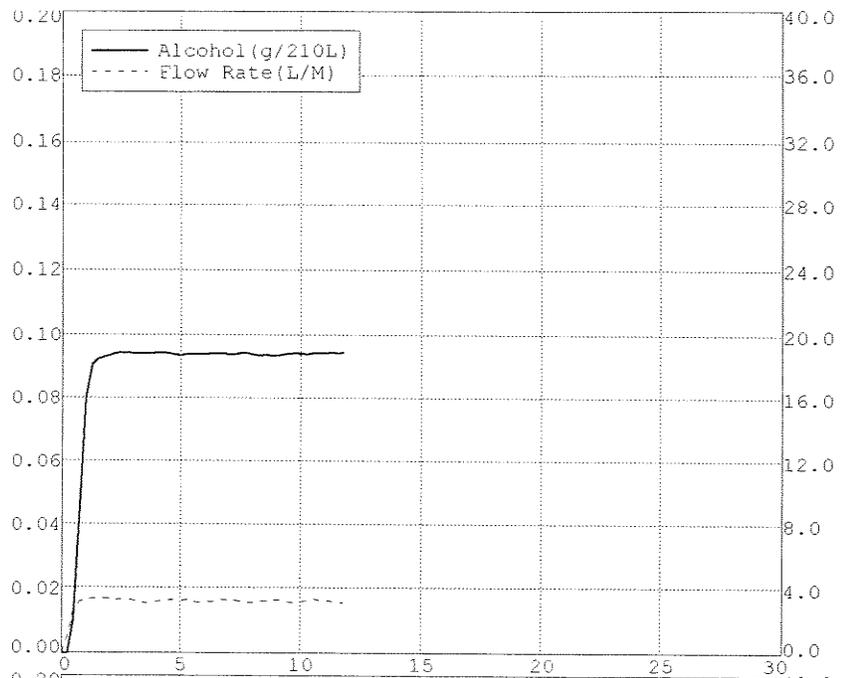

*Charles B Geisler #241*