

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/08/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:55
INTERNAL STANDARD	VERIFIED	20:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:55
BLANK TEST	0.00	20:56
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	20:57
BLANK TEST	0.00	20:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:58
BLANK TEST	0.00	20:59

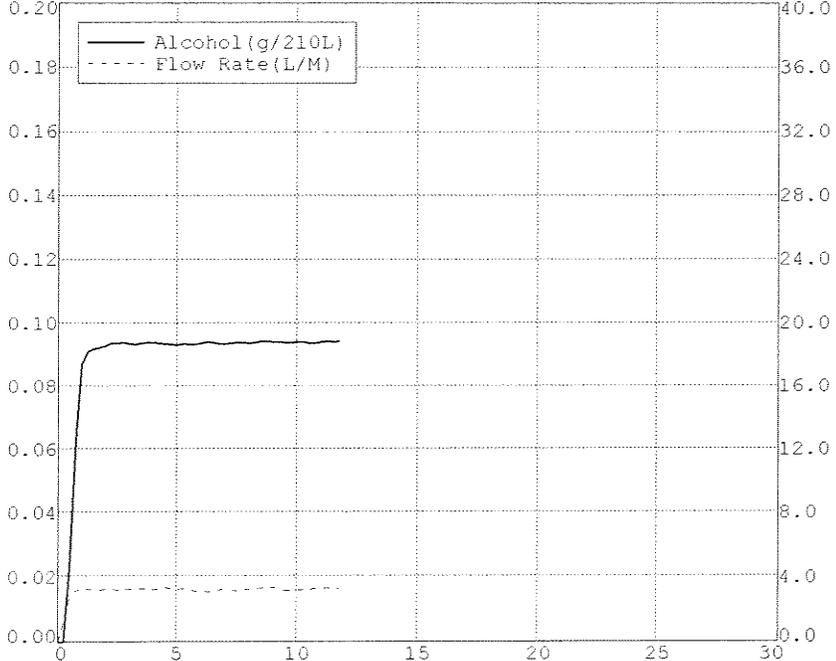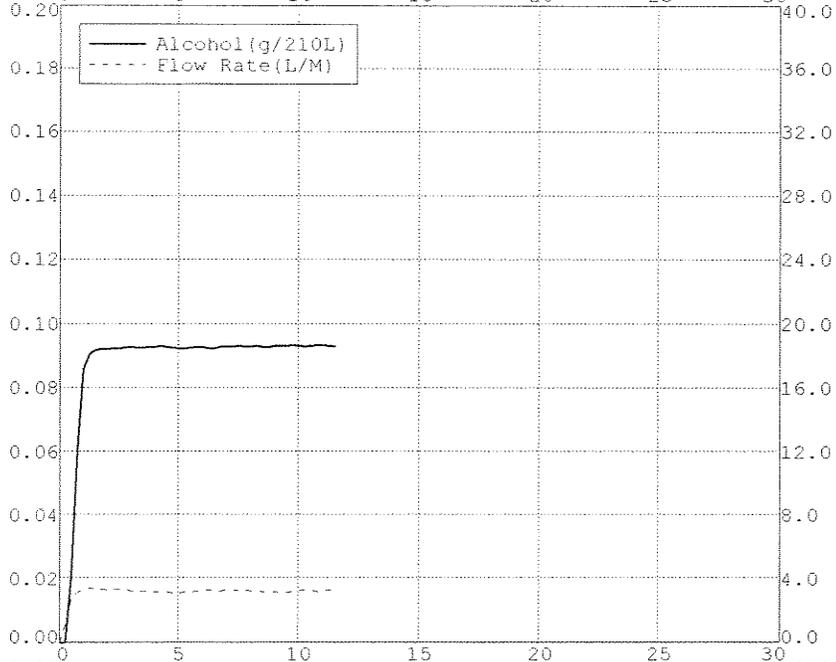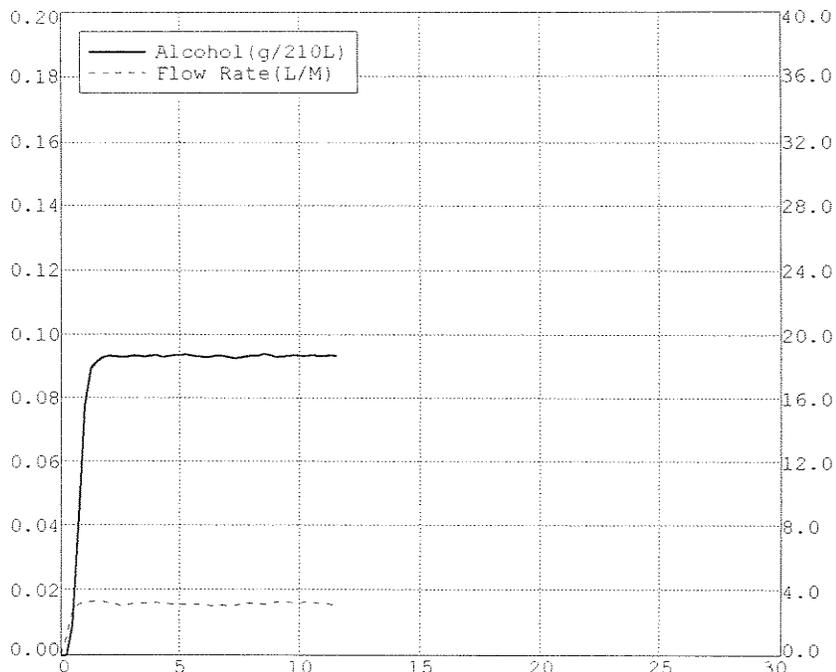

Sp. Ct. - 13. 0.17 #291