

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/13/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:54
INTERNAL STANDARD	VERIFIED	14:54
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	14:54
BLANK TEST	0.00	14:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:55
BLANK TEST	0.00	14:56
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	14:57
BLANK TEST	0.00	14:58

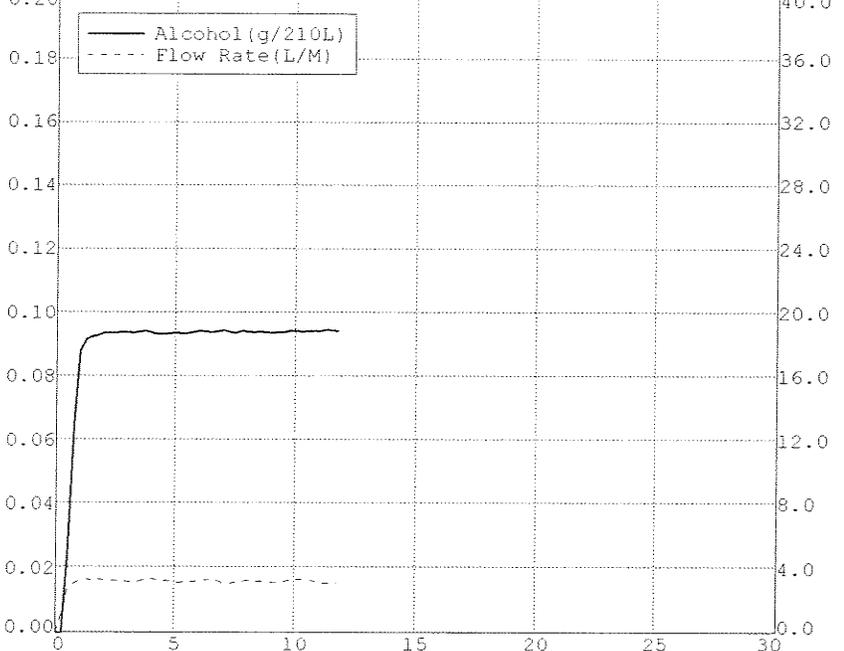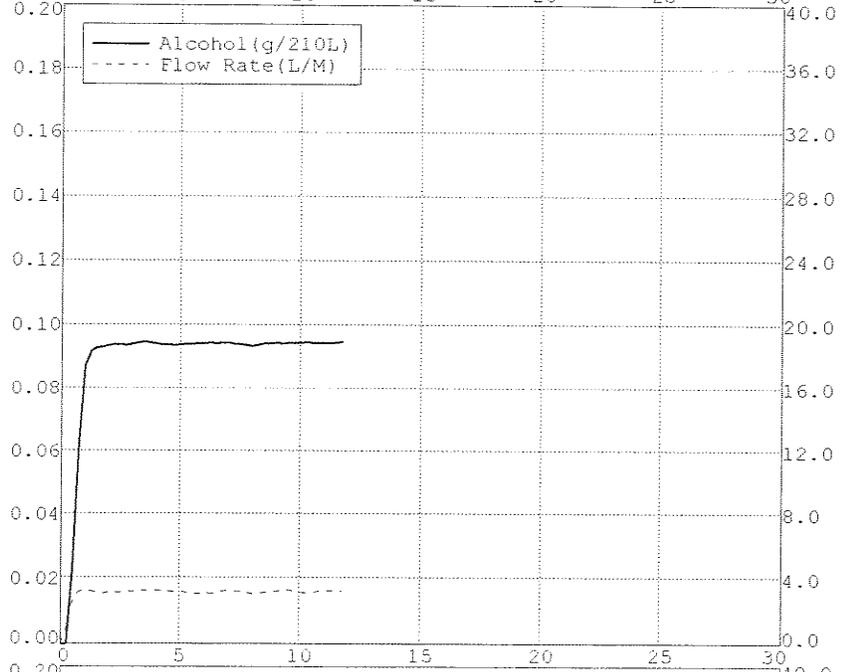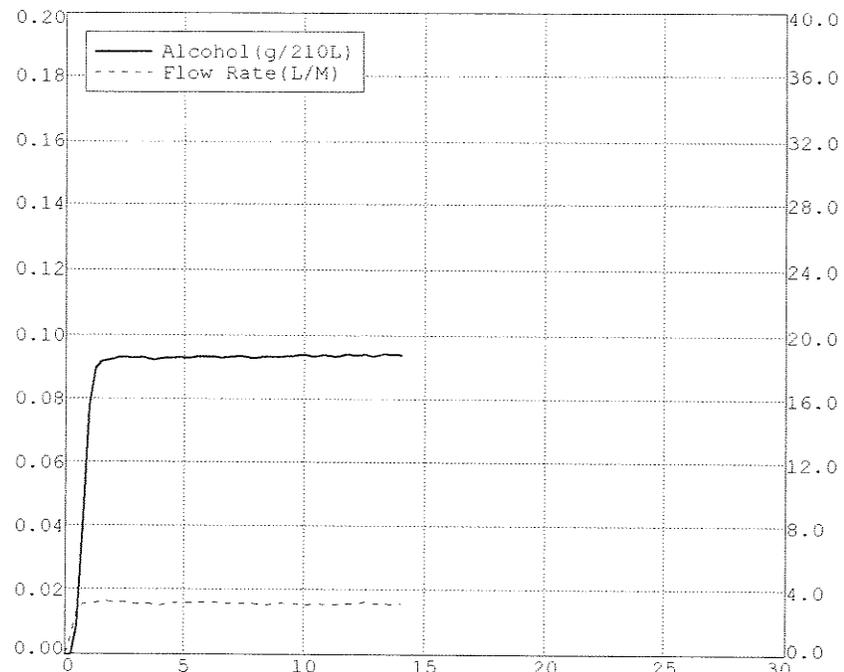

Ch. B. Geisler #248