

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 09/19/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:32
INTERNAL STANDARD	VERIFIED	04:32
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	04:32
BLANK TEST	0.00	04:33
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	04:34
BLANK TEST	0.00	04:35
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	04:35
BLANK TEST	0.00	04:36

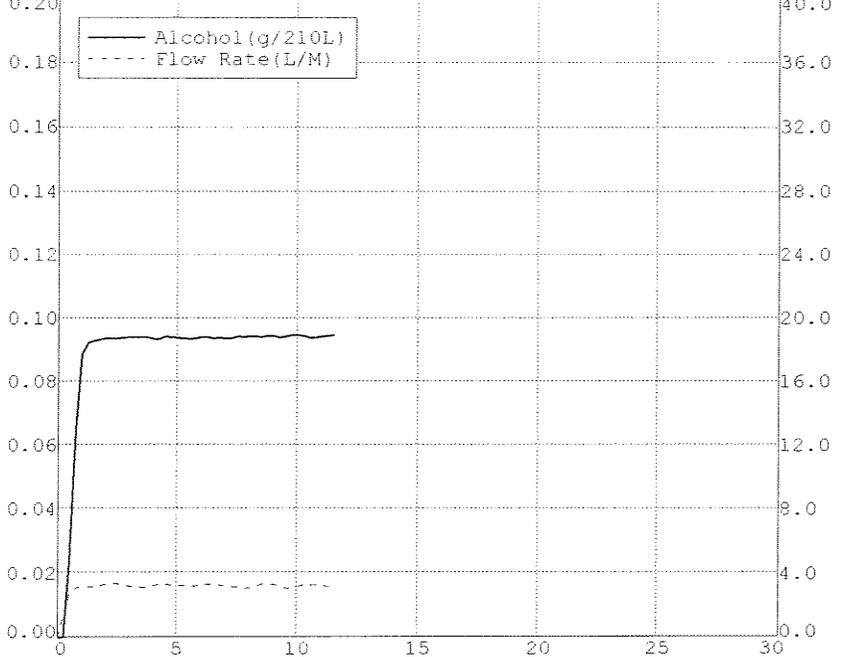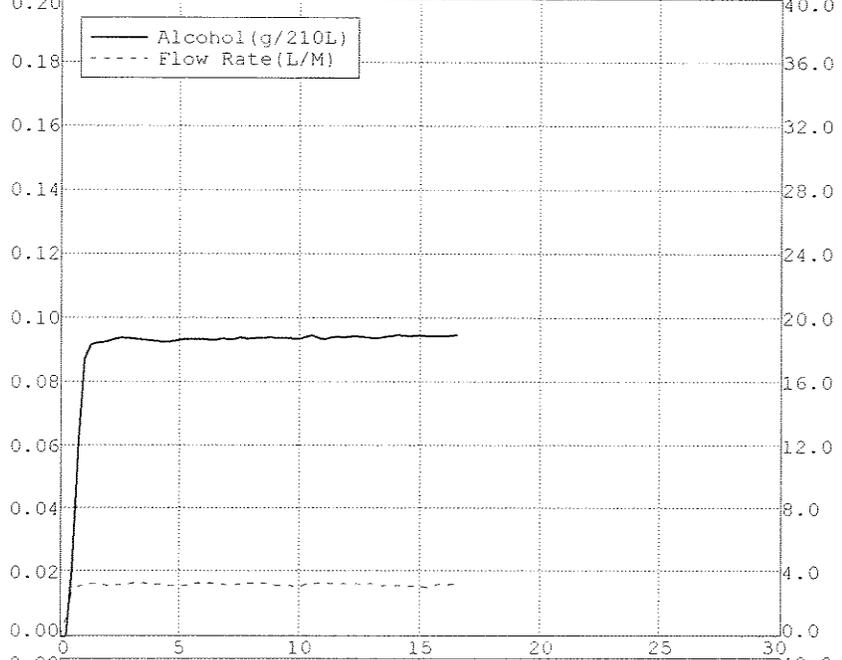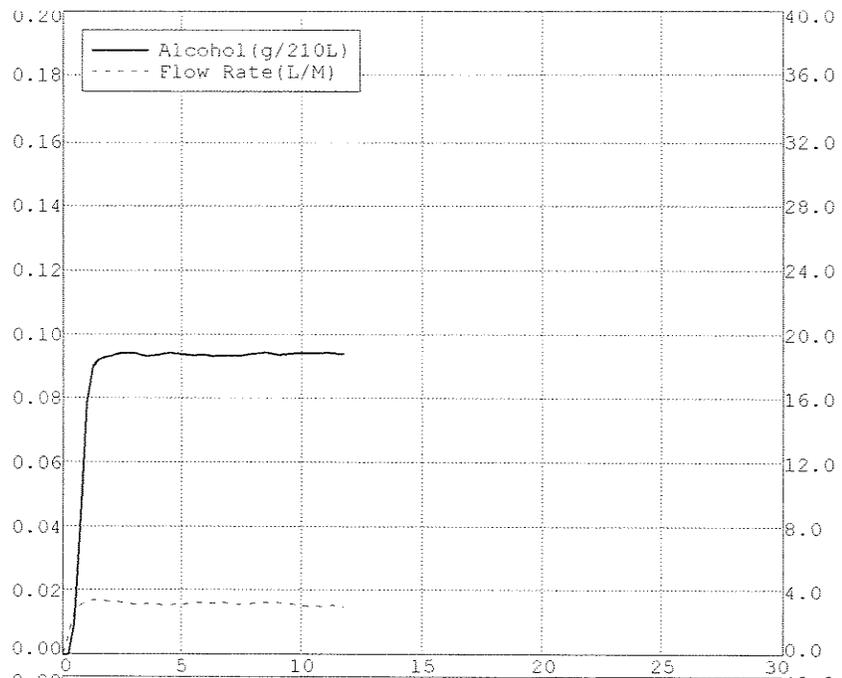

*Handwritten signature: JG CB-BS CB #241*