

SUPERVISOR TEST


WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/25/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:22
INTERNAL STANDARD	VERIFIED	01:22
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:22
BLANK TEST	0.00	01:23
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:24
BLANK TEST	0.00	01:24
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:25
BLANK TEST	0.00	01:26

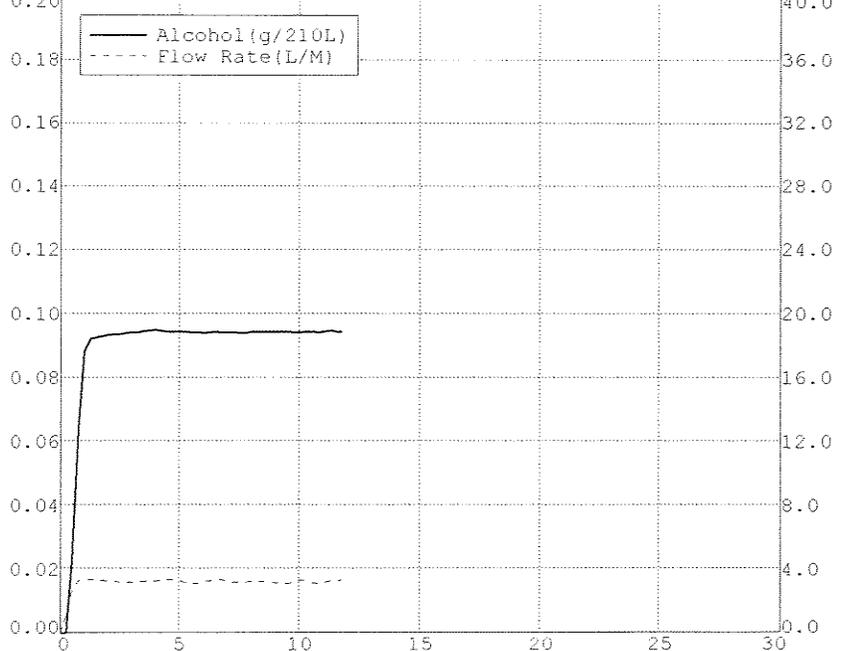

Charles B Geisler #245