

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 10/30/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:12
INTERNAL STANDARD	VERIFIED	13:12
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	13:12
BLANK TEST	0.00	13:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:13
BLANK TEST	0.00	13:14
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	13:14
BLANK TEST	0.00	13:15

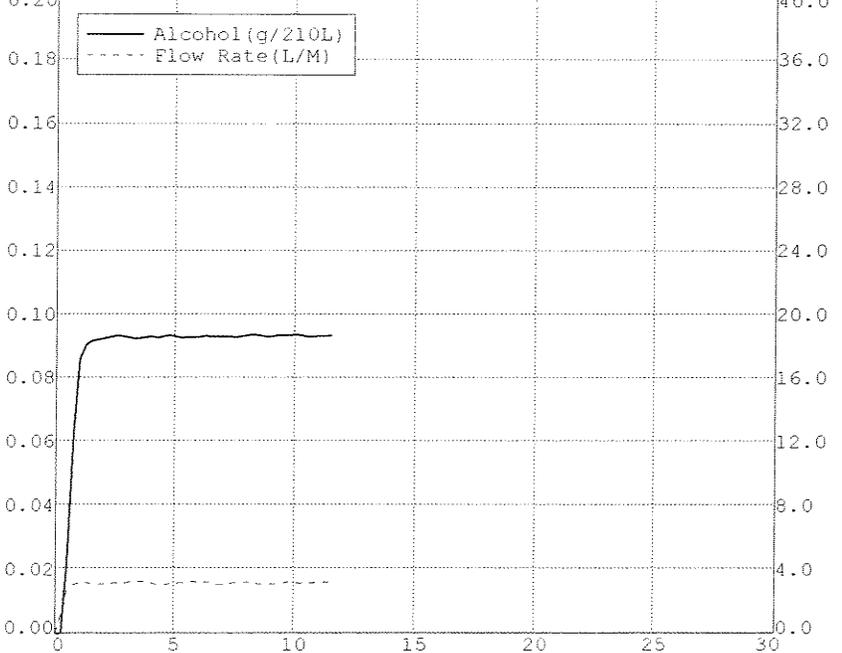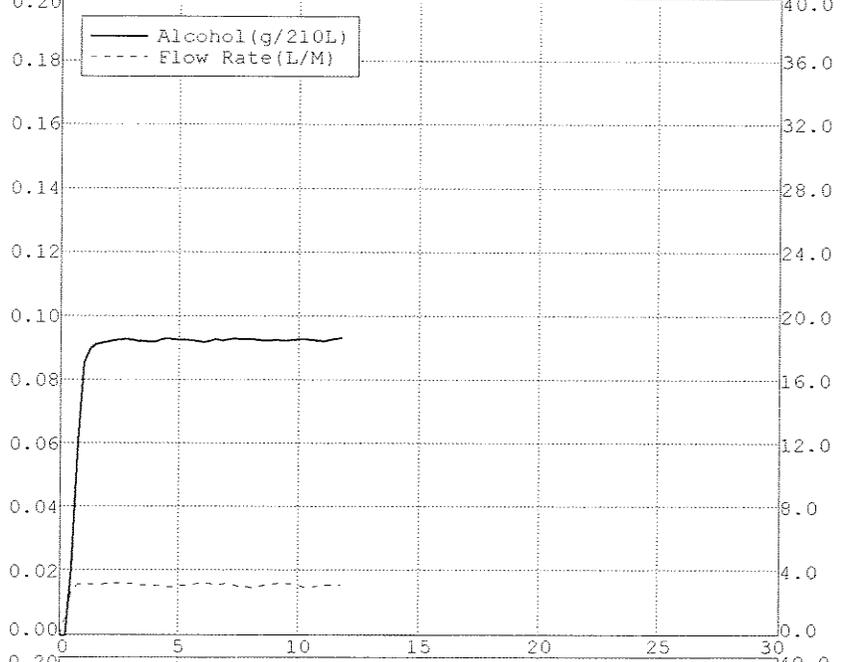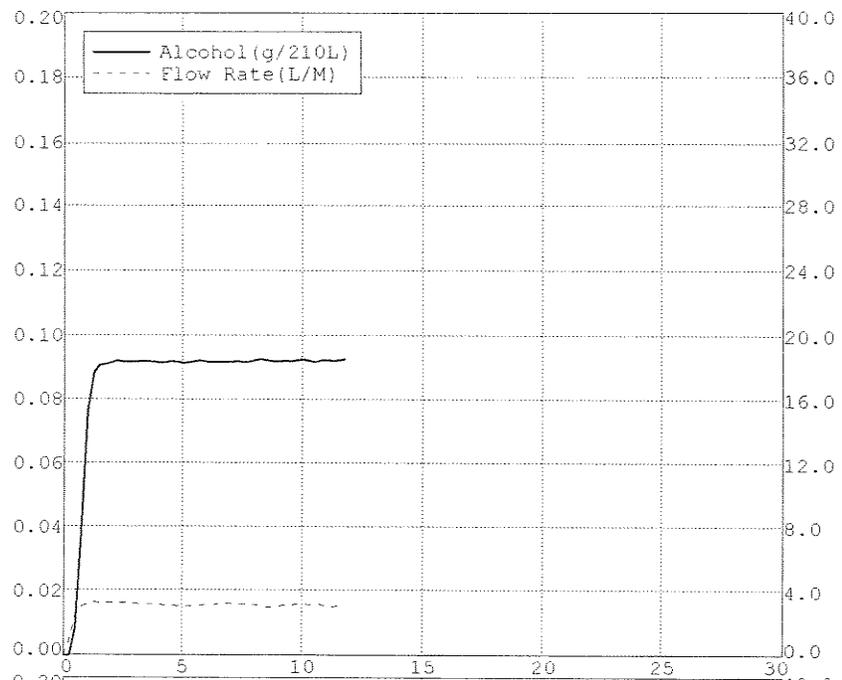

*Ch. B. Geisler #241*