

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 11/01/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:51
INTERNAL STANDARD	VERIFIED	16:51
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	16:52
BLANK TEST	0.00	16:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:53
BLANK TEST	0.00	16:54
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	16:54
BLANK TEST	0.00	16:55

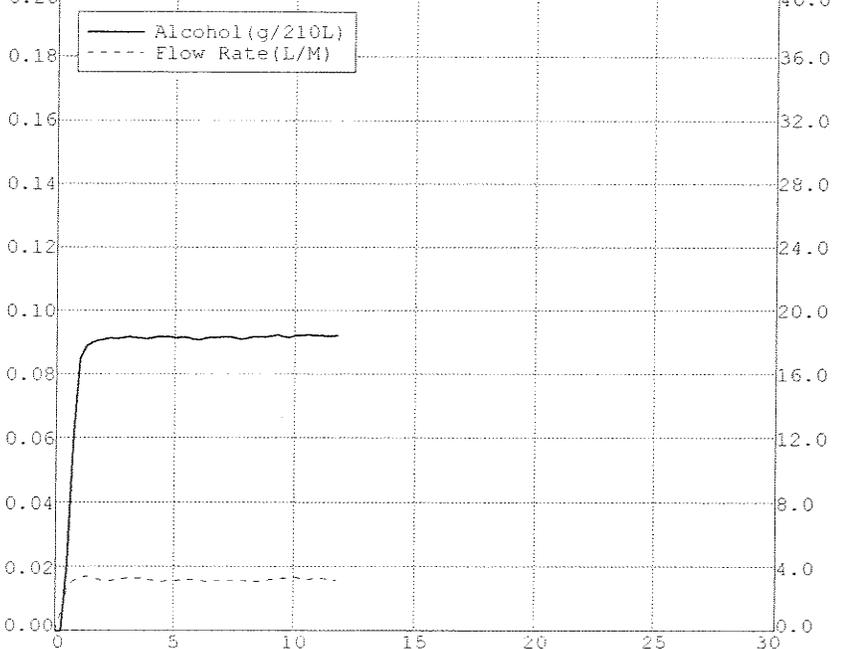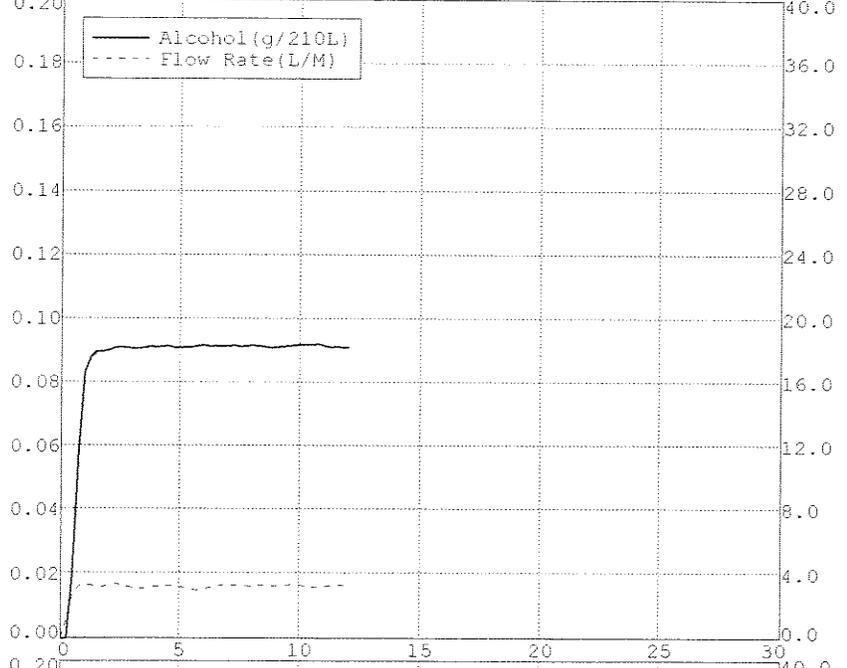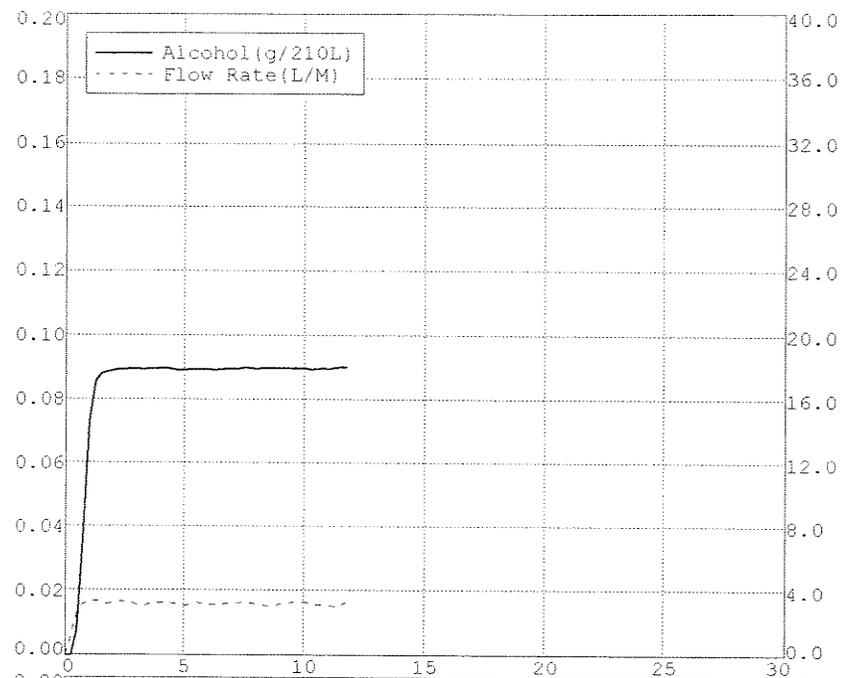

*Charles B. Geisler* #207