

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 11/27/2017

OPERATOR NAME:  
TYLER J MORSE  
Permit #: 41959  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:15
INTERNAL STANDARD	VERIFIED	08:15
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:15
BLANK TEST	0.00	08:16
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:16
BLANK TEST	0.00	08:17
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.09	08:18
BLANK TEST	0.00	08:19

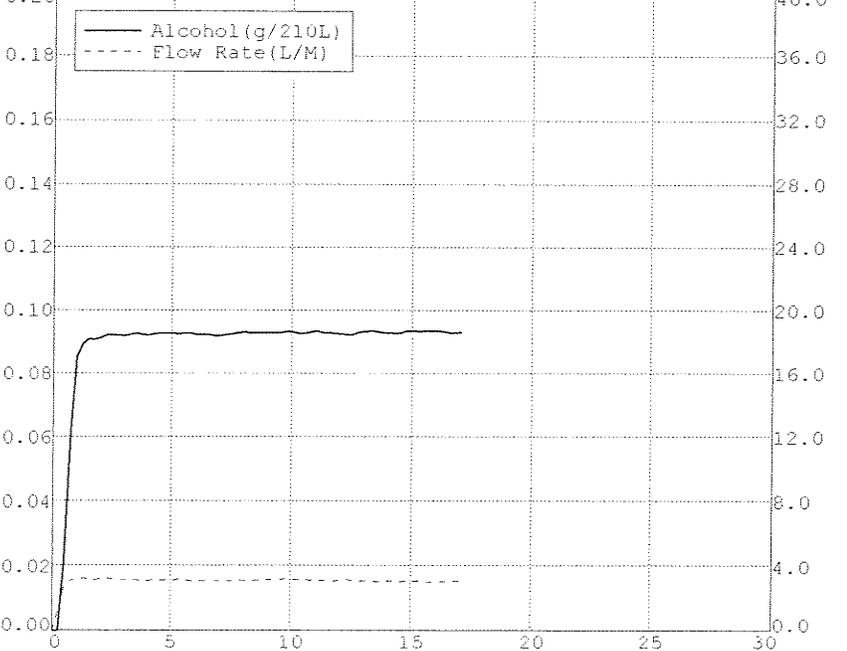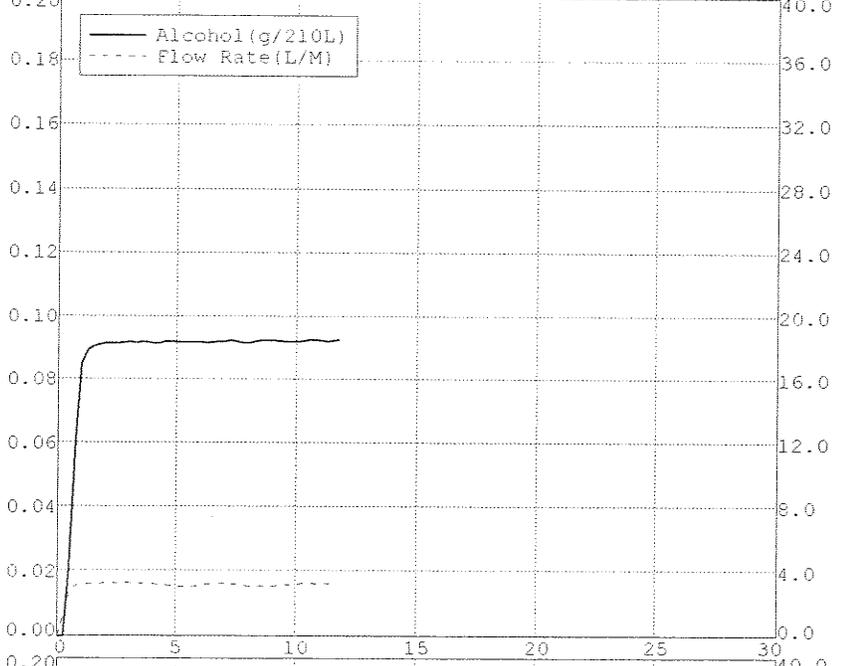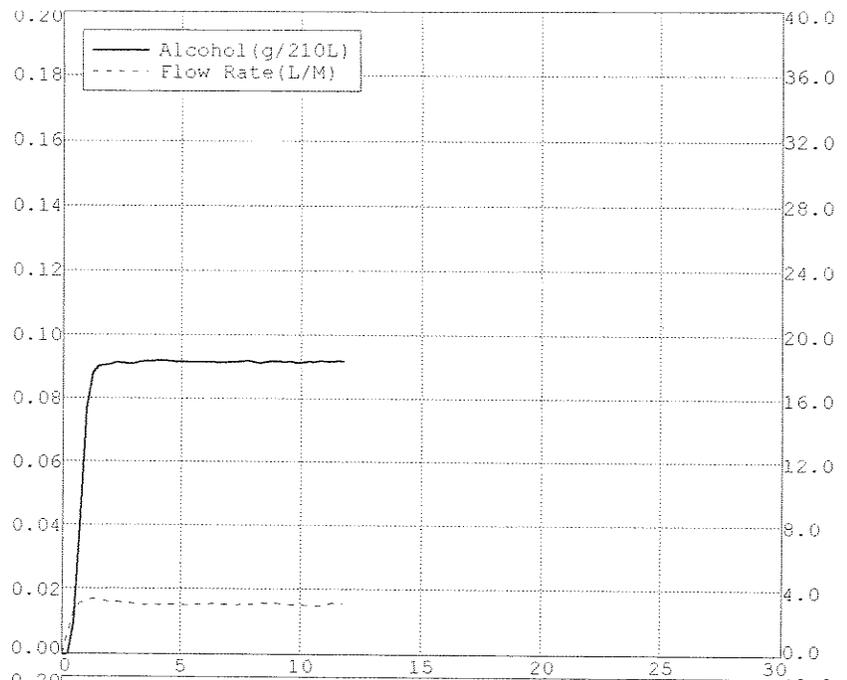

*DS JV #447*