

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 12/16/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:08
INTERNAL STANDARD	VERIFIED	02:08
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:09
BLANK TEST	0.00	02:09
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	02:10
BLANK TEST	0.00	02:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:11
BLANK TEST	0.00	02:12

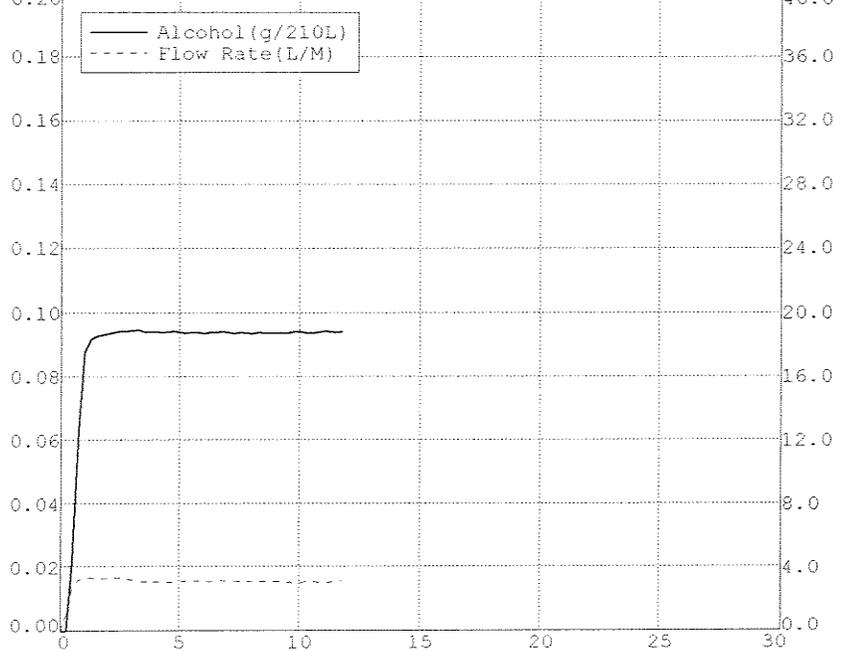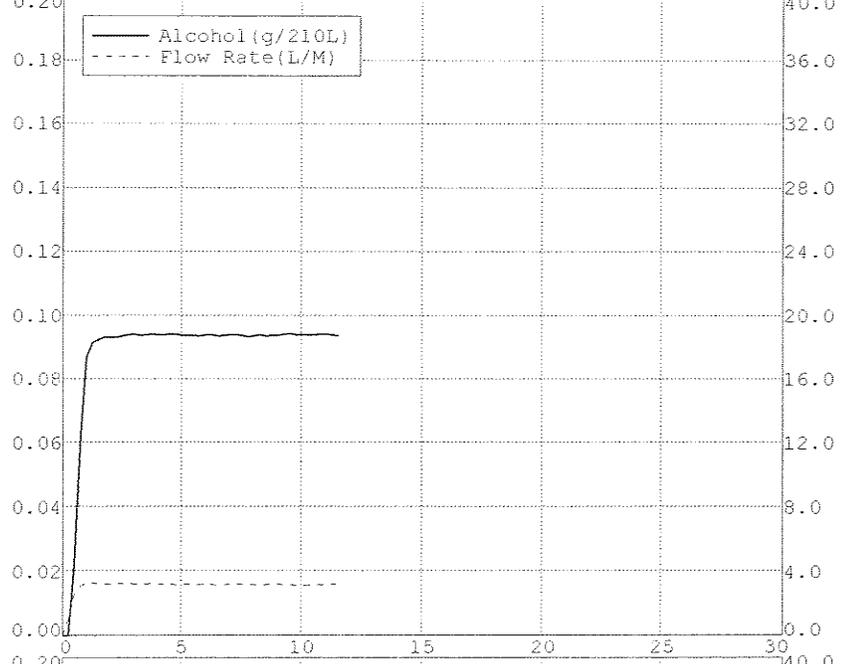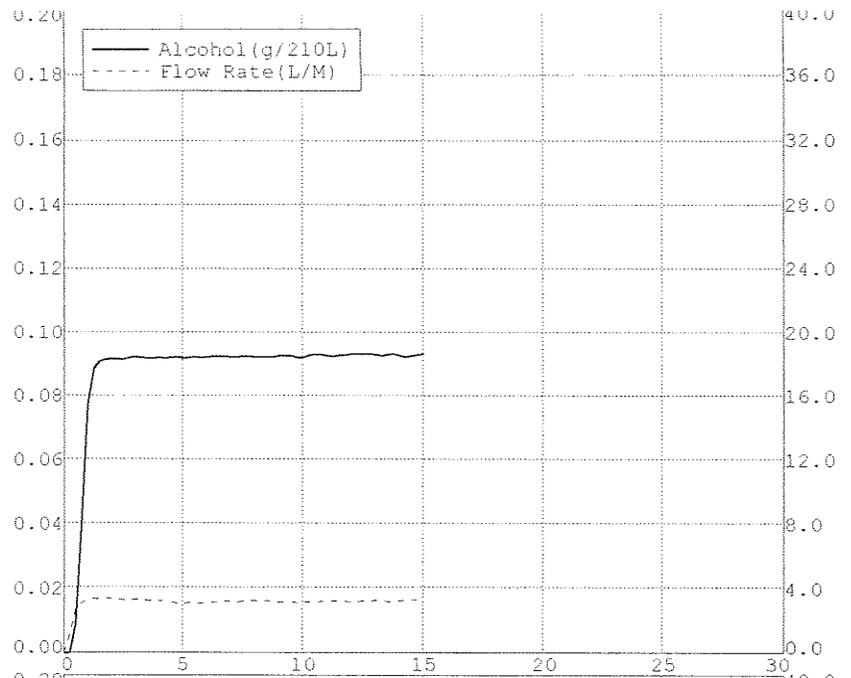

Spec 21-20- [Signature] #241