

SUPERVISOR TEST



WARREN COUNTY  
 SHERRIF'S OFFICE  
 DATAMASTER dmt: 144506

Date: 03/27/2017

OPERATOR NAME:  
 RALPH J BARTLETT  
 Permit #: 26222  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 16380

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:47
INTERNAL STANDARD	VERIFIED	00:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:47
BLANK TEST	0.00	00:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:49
BLANK TEST	0.00	00:50
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:50
BLANK TEST	0.00	00:51

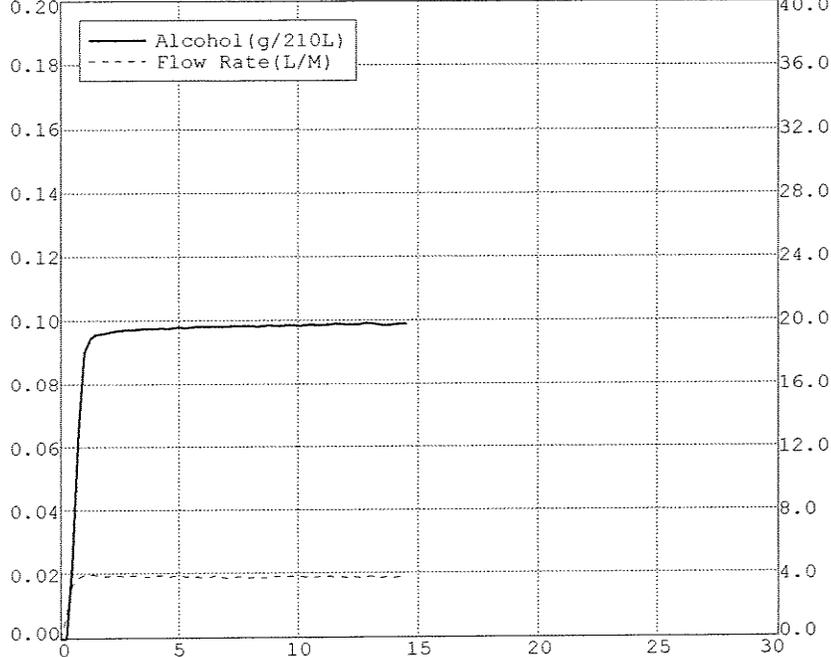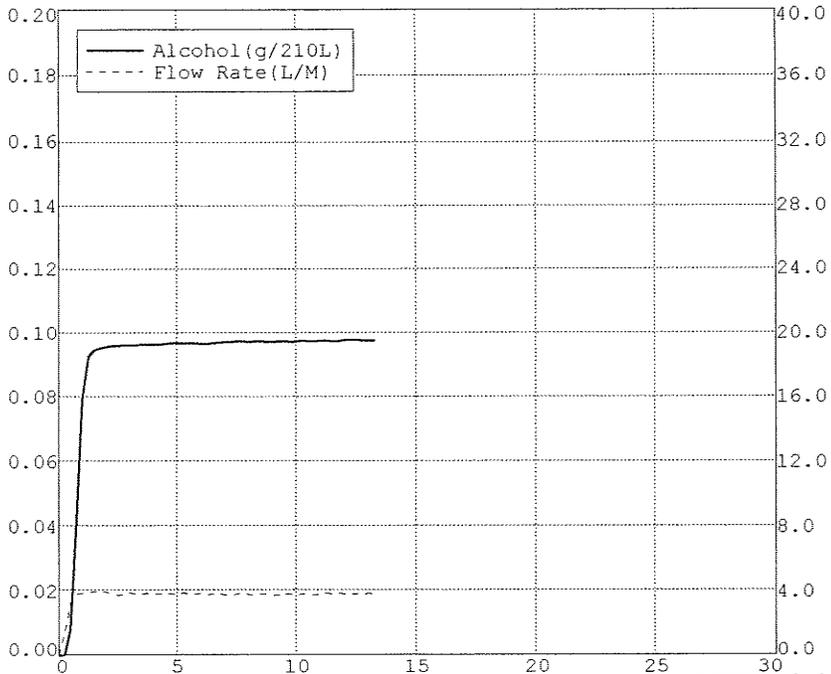

Sus Rly Bartlett WOSO #162  
 03-27-17