

SUPERVISOR TEST

WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506


Date: 04/28/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:01
INTERNAL STANDARD	VERIFIED	00:01
REFERENCE STANDARD TEMP	33.93c	
REFERENCE STANDARD	0.09	00:02

Filter 3 Won't Zero

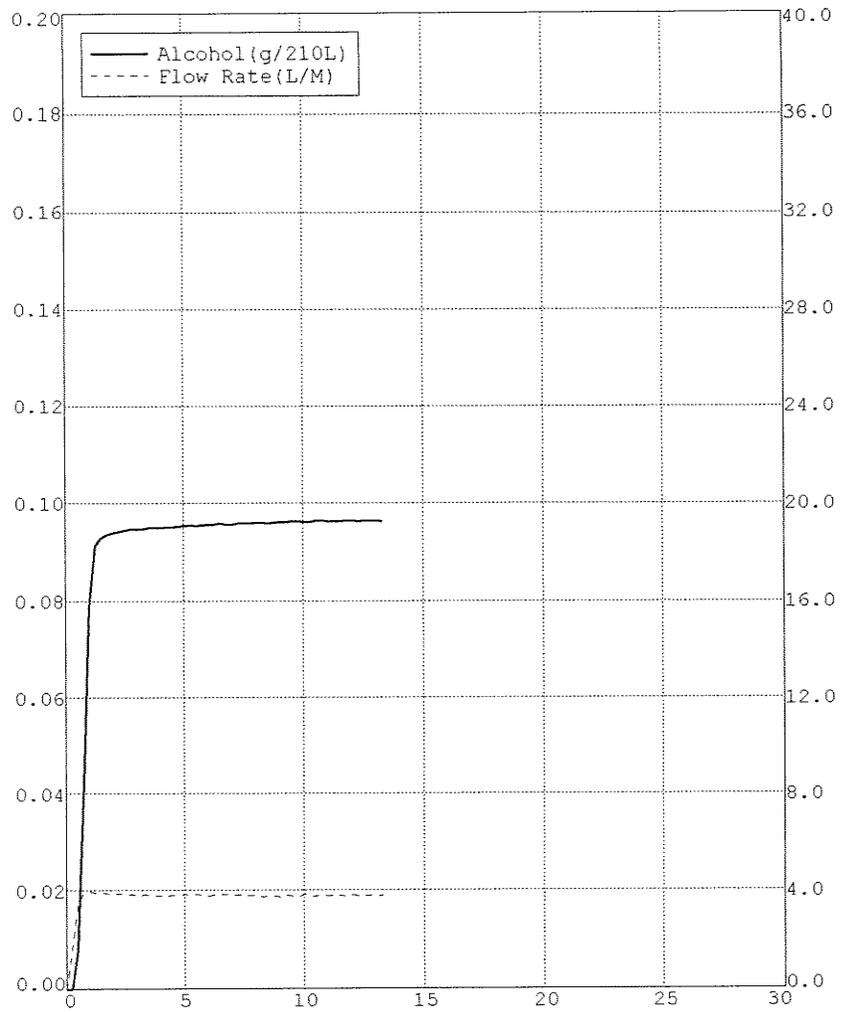

Sgt. M. D. [Signature] 4/28/17

SUPERVISOR TEST




WARREN COUNTY
 SHERRIF'S OFFICE
 DATAMASTER dmt: 144506

Date: 04/28/2017

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:14
INTERNAL STANDARD	VERIFIED	00:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:14
BLANK TEST	0.00	00:15
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	00:15
BLANK TEST	0.00	00:16
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	00:17
BLANK TEST	0.00	00:18

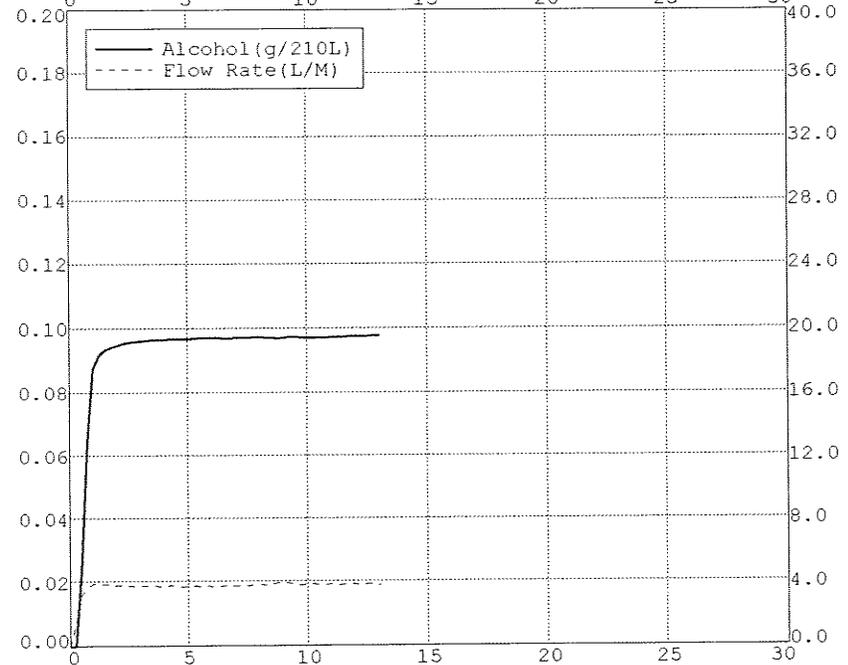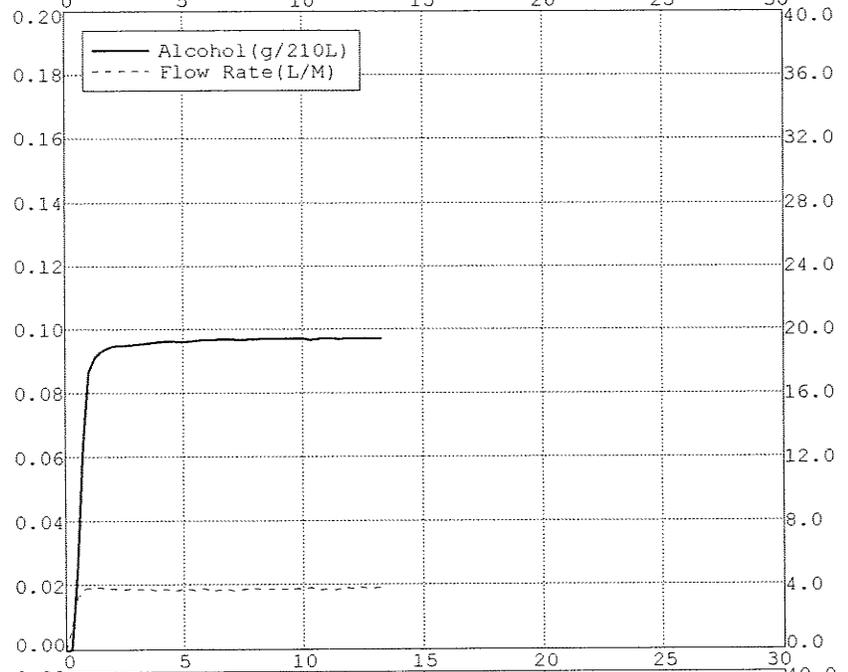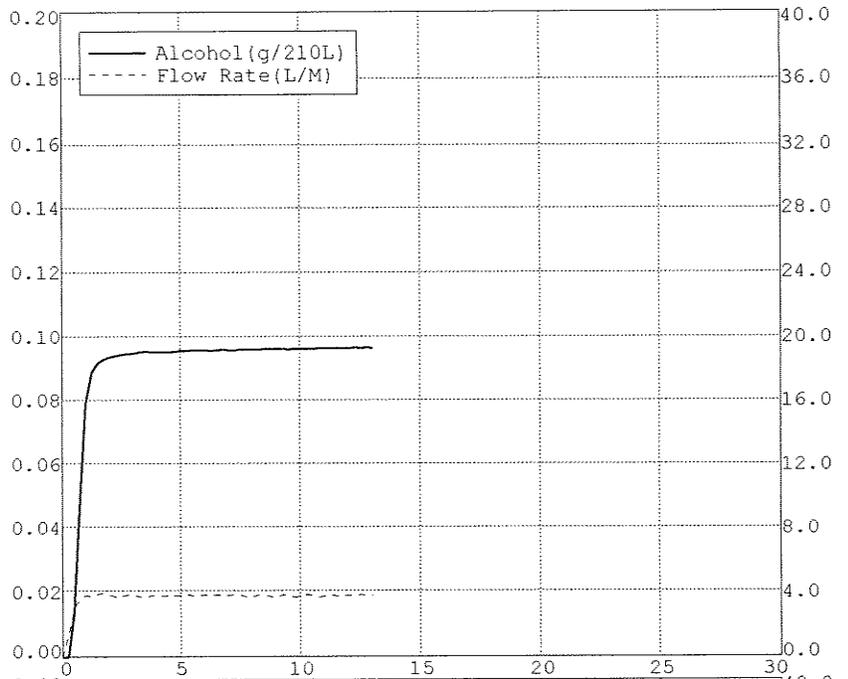

See Mr. B. G. #218 4/28/17