

SOLUTION CHANGE




WARREN COUNTY
SHERRIF'S OFFICE
DATAMASTER dmt: 144506

Date: 05/02/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:53
INTERNAL STANDARD	VERIFIED	00:53
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:53
BLANK TEST	0.00	00:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:54
BLANK TEST	0.00	00:55
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	00:55
BLANK TEST	0.00	00:56

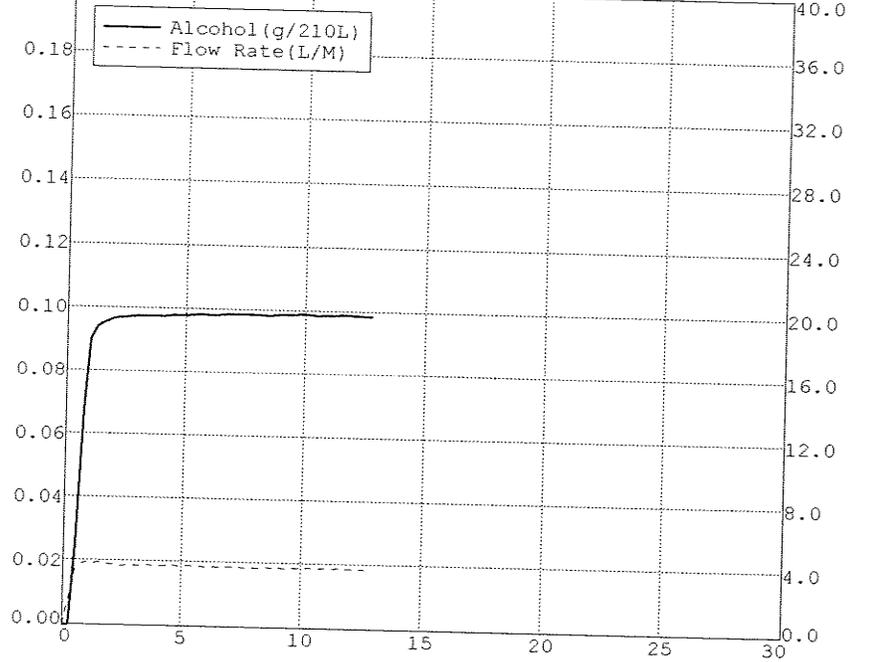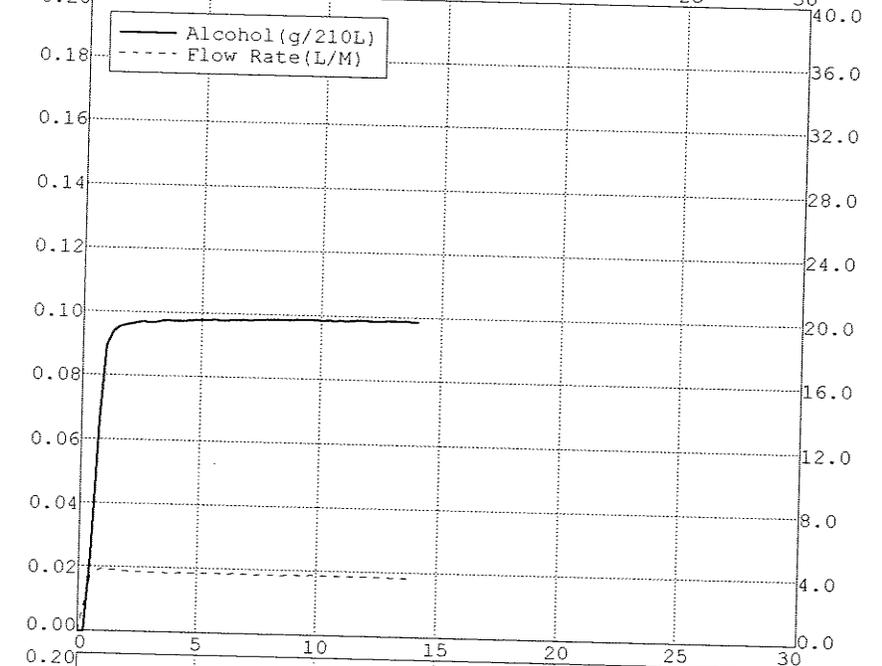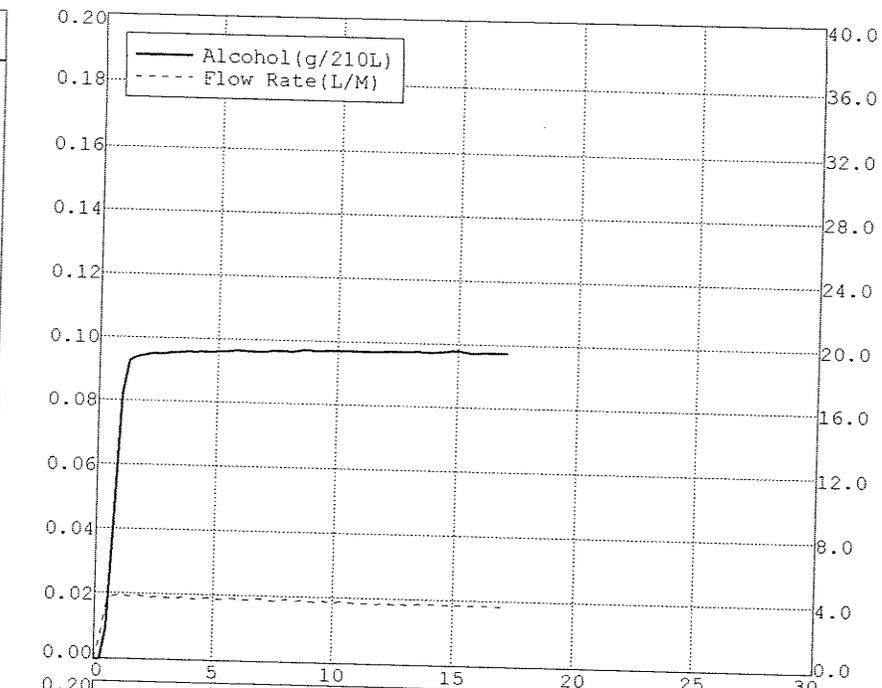

Charles B. Geisler #246