

SUPERVISOR TEST




WARREN COUNTY
 SHERRIF'S OFFICE
 DATAMASTER dmt: 144506

Date: 05/15/2017

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:58
INTERNAL STANDARD	VERIFIED	09:59
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	09:59
BLANK TEST	0.00	10:00
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	10:00
BLANK TEST	0.00	10:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:01
BLANK TEST	0.00	10:02

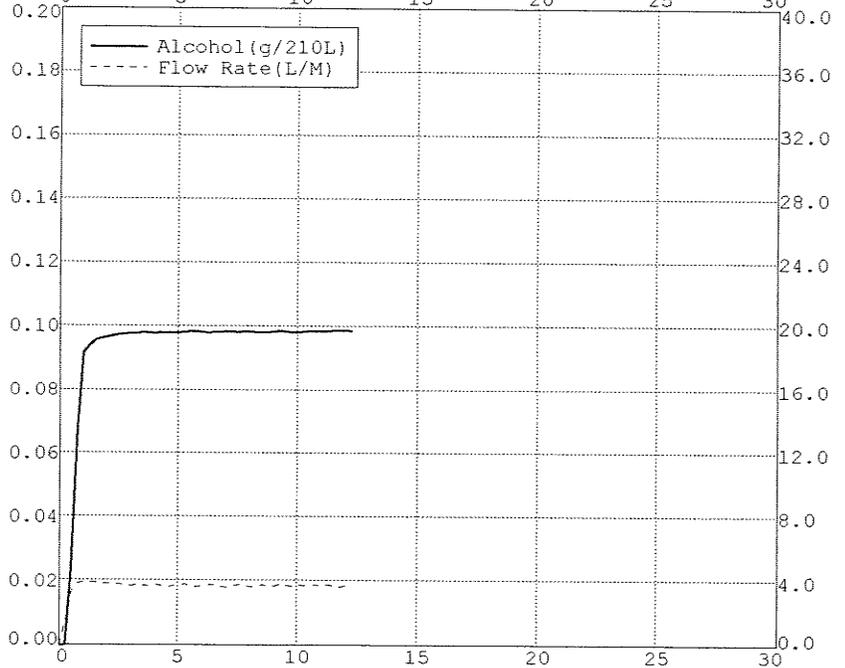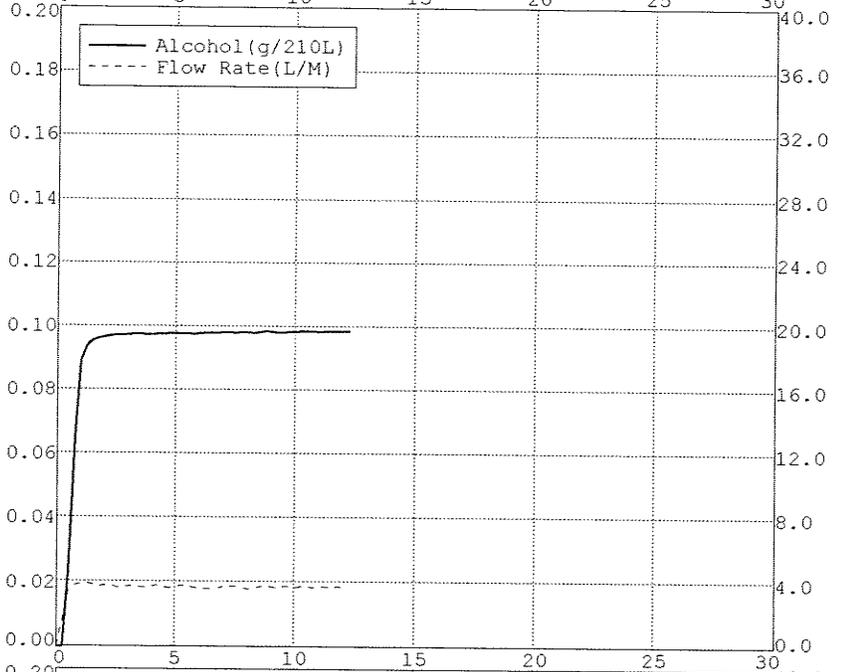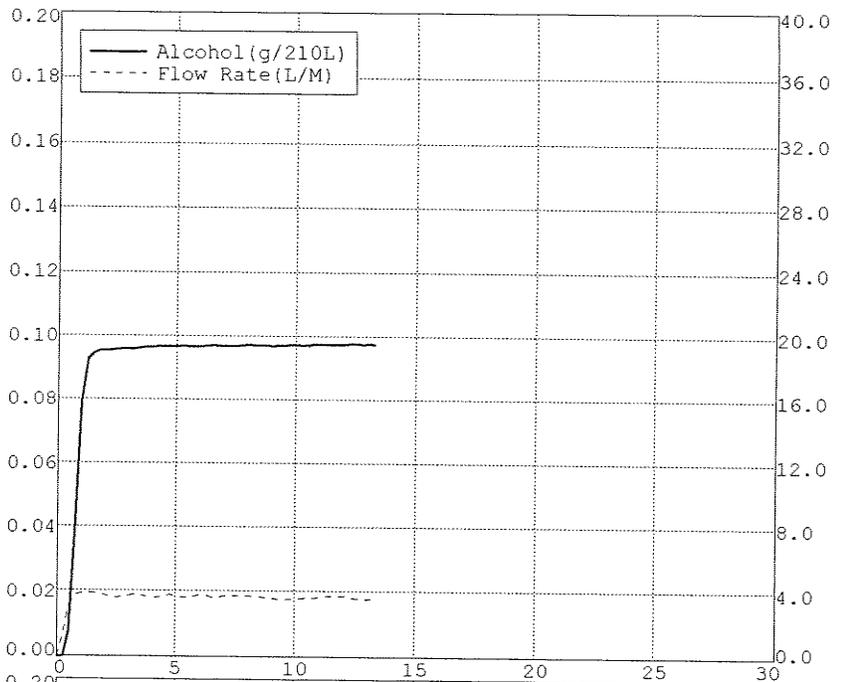

C. B. Geisler 5/15/17