

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 05/29/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:40
INTERNAL STANDARD	VERIFIED	23:41
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	23:41
BLANK TEST	0.00	23:42
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	23:42
BLANK TEST	0.00	23:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:43
BLANK TEST	0.00	23:44

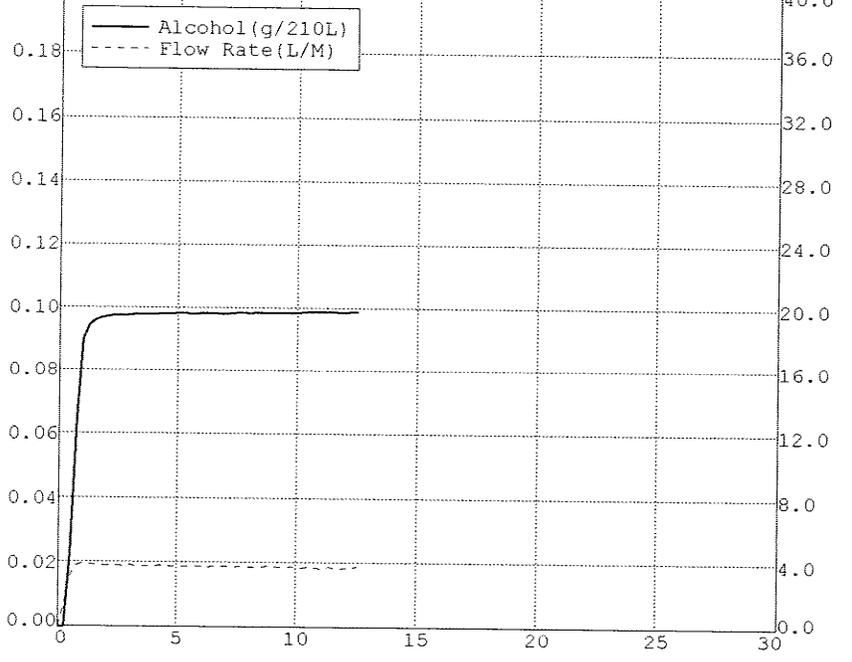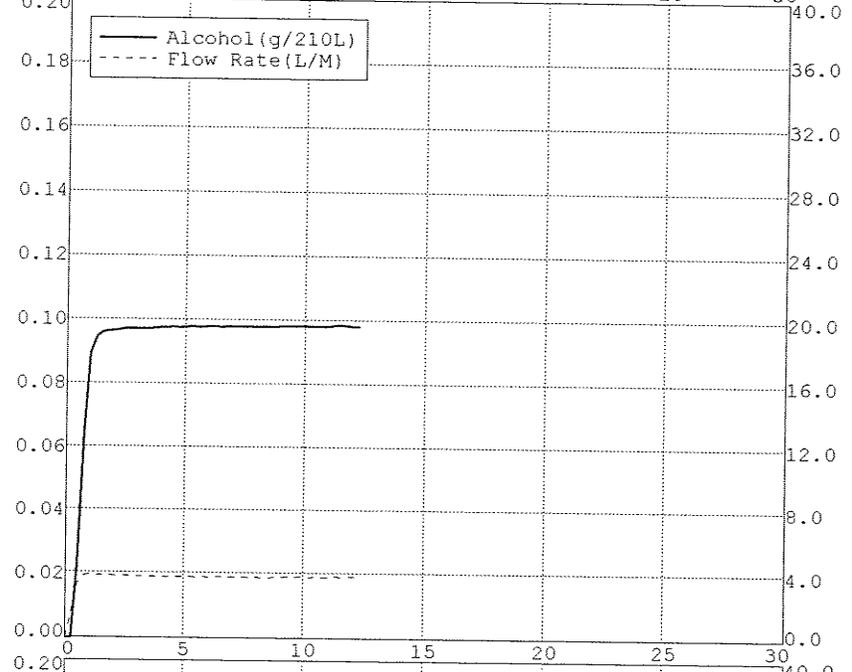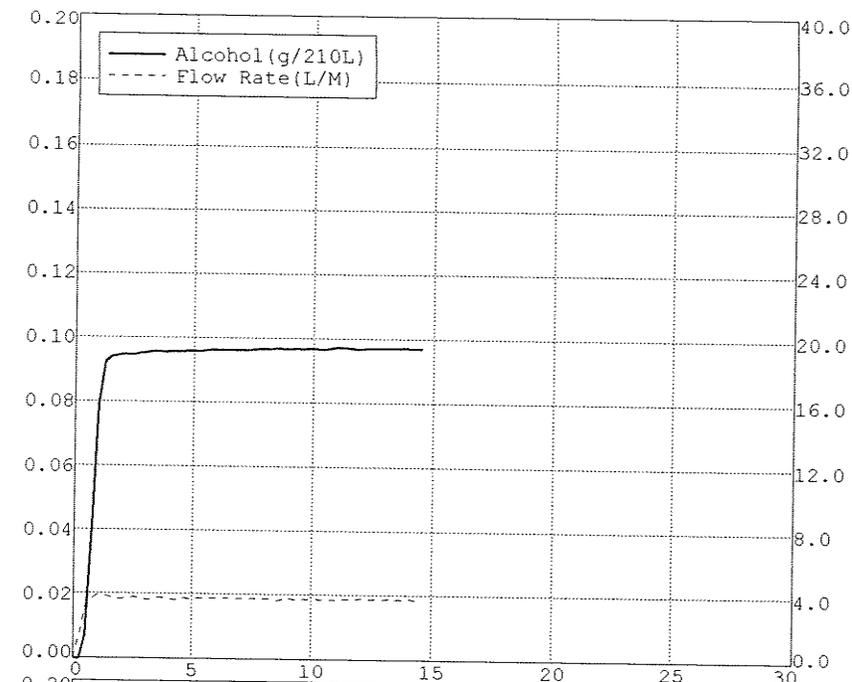

Sup. Chd. B. G. #245