

SOLUTION CHANGE




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 06/03/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:01
INTERNAL STANDARD	VERIFIED	03:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:02
BLANK TEST	0.00	03:03
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	03:03
BLANK TEST	0.00	03:04
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	03:04
BLANK TEST	0.00	03:05

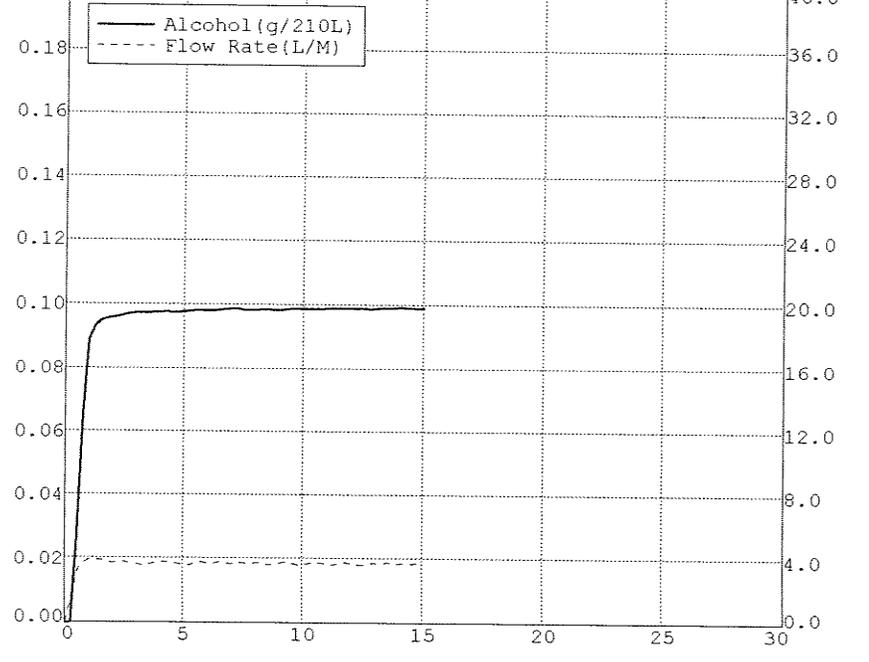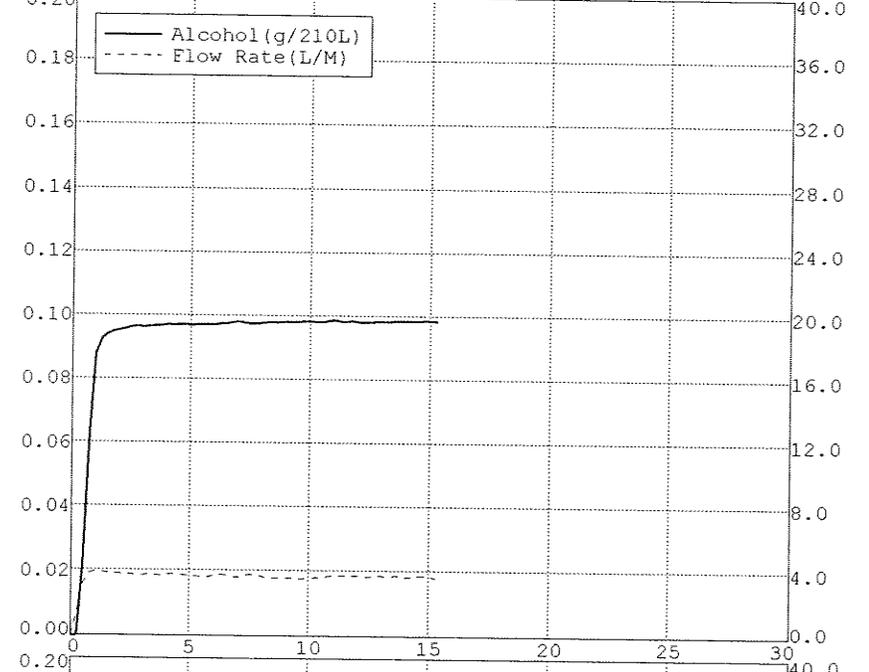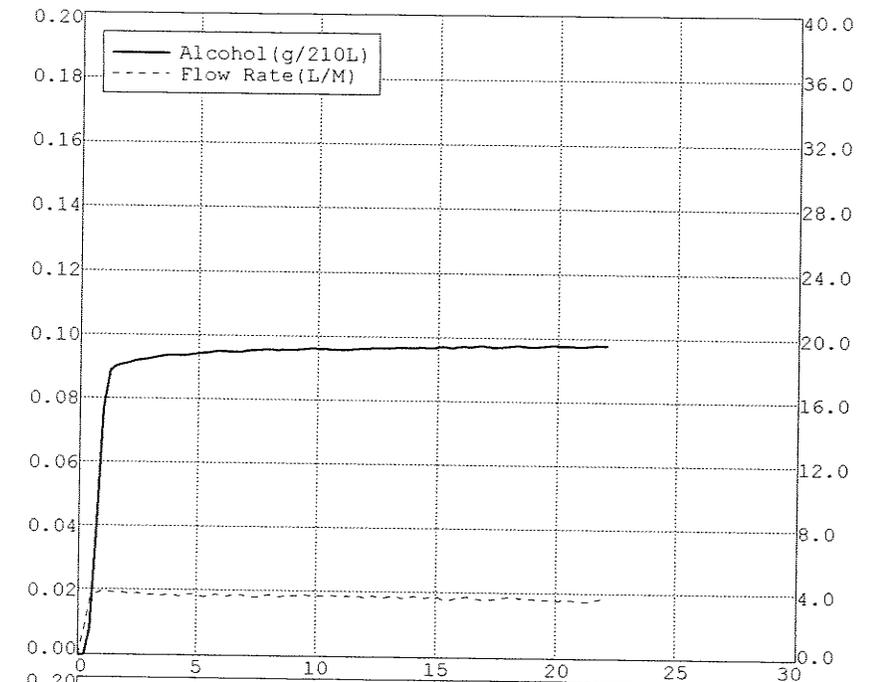

*Charles B. Geisler #201*